


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

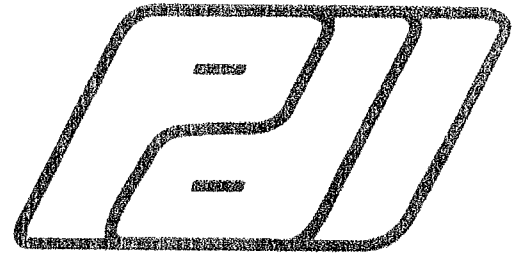

Serial No: 80150 Temperature: 23.1 °C

Model: PE Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

936.7 g's/volt

R²: 0.999968 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 31Jul2026

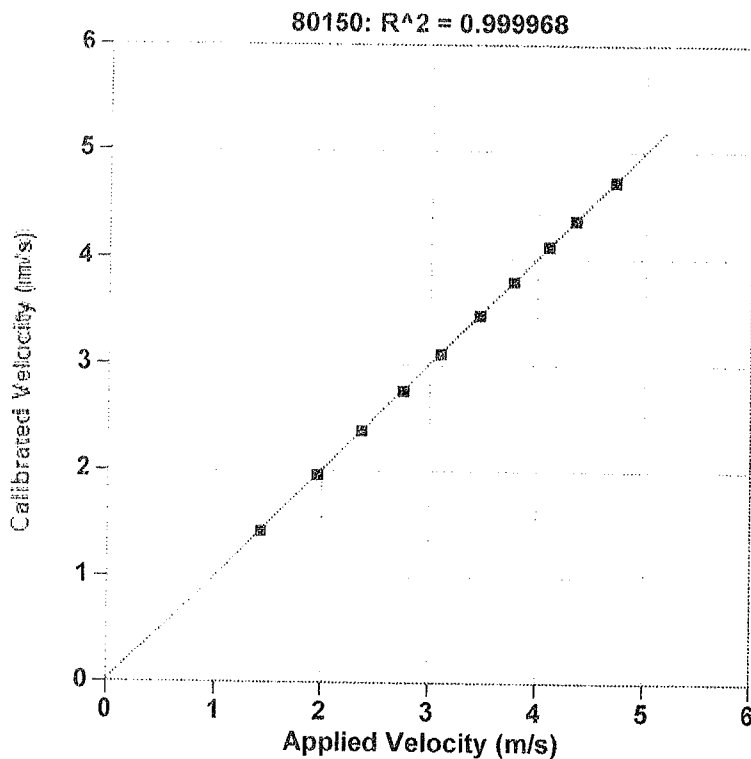

Reference Velocity	S/N 80150 Velocity
m/s	m/s
1.432	1.426
1.964	1.959
2.379	2.375
2.755	2.746
3.099	3.099
3.464	3.461
3.773	3.780
4.103	4.111
4.350	4.355
4.718	4.716
Maximum Acceleration: 1033 g's	