

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K10119 Temperature: 22.4 °C

Model: KICHER PR Humidity: 38%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

355.1 mv/5000g


(71.0 μ v/g)

R²: 0.999973 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 01Aug2026

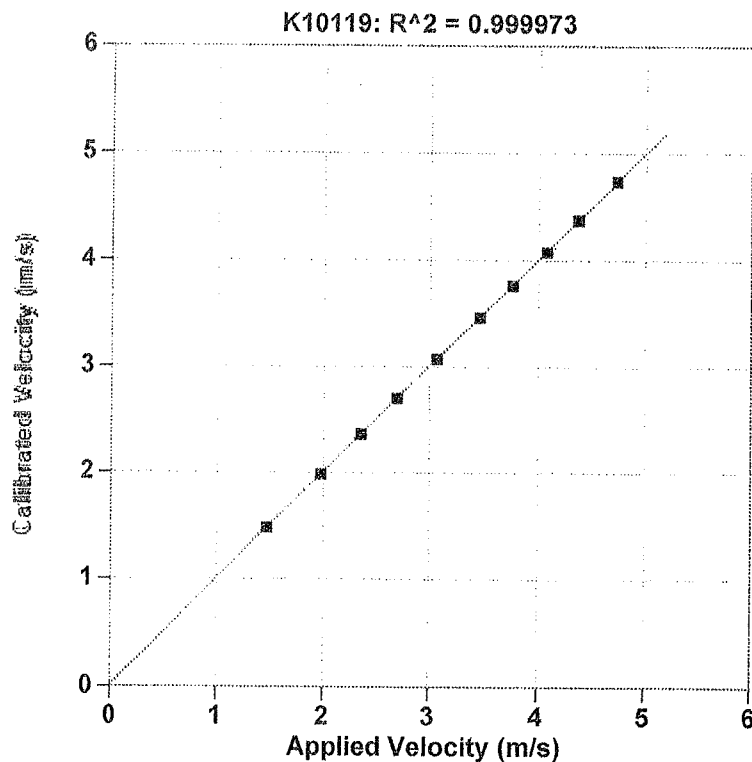

Reference Velocity	S/N K10119 Velocity
m/s	m/s
1.469	1.469
1.979	1.976
2.360	2.353
2.699	2.693
3.067	3.067
3.460	3.459
3.760	3.759
4.075	4.070
4.367	4.372
4.725	4.736

Maximum Acceleration: 1034 g's