

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.




Serial No: K10717 Temperature: 22.4 °C
Model: KICHER PR Humidity: 38%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

453.1 mv/5000g
(90.6 µv/g)
R^2: 0.999958 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 01Aug2026

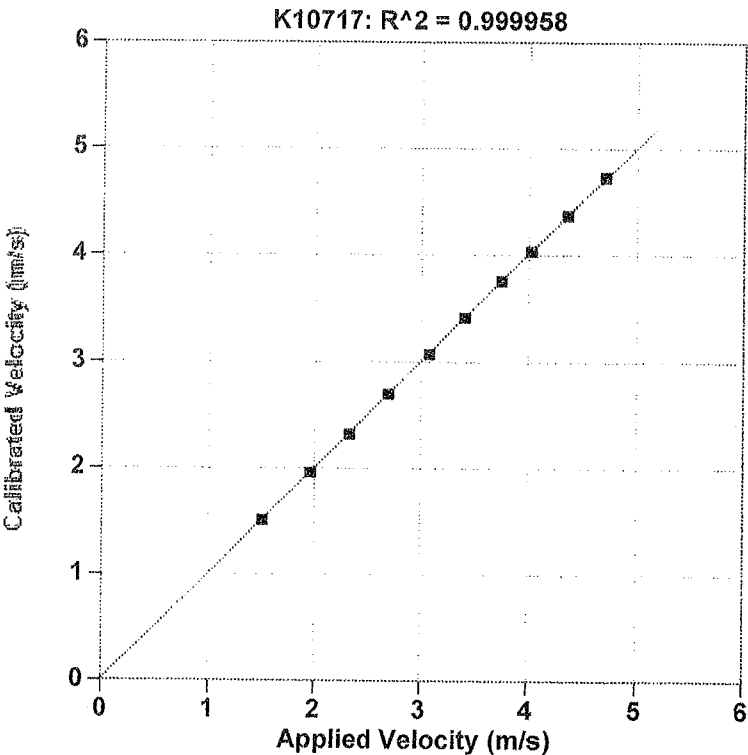

Reference Velocity	S/N K10717 Velocity
m/s	m/s
1.515	1.511
1.964	1.958
2.325	2.319
2.698	2.693
3.078	3.072
3.414	3.410
3.752	3.750
4.029	4.028
4.362	4.366
4.710	4.725

Maximum Acceleration: 1031 g's