


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

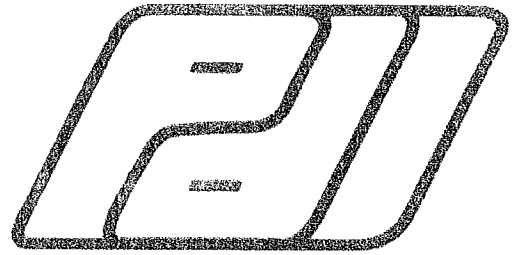

Serial No: K10808 Temperature: 23.7 °C

Model: KICHER PR Humidity: 43%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

429.0 mv/5000g

(85.8 μ v/g)

R²: 0.999956 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 10Aug2026

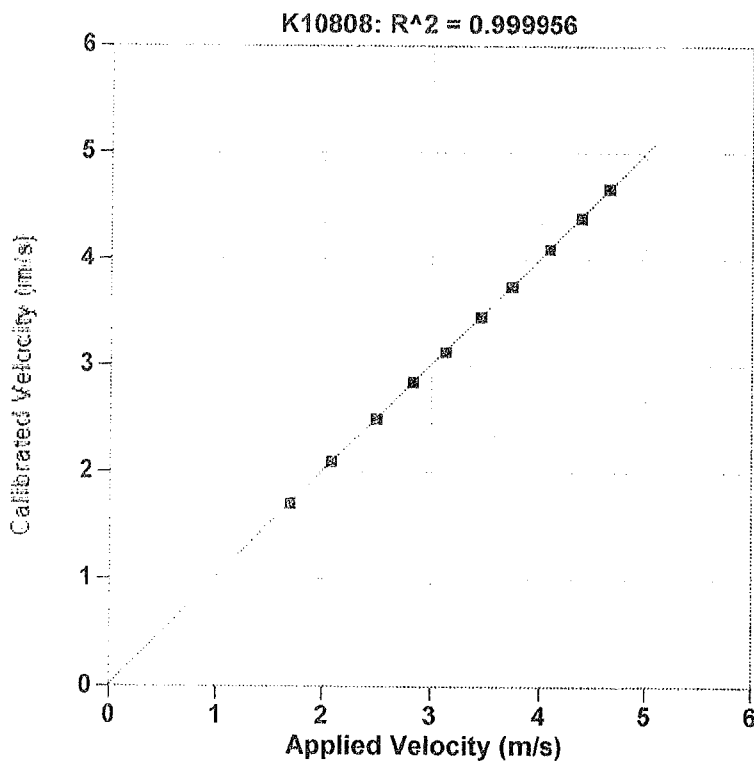

Reference Velocity	S/N K10808 Velocity
m/s	m/s
1.700	1.697
2.082	2.088
2.492	2.487
2.834	2.832
3.129	3.119
3.459	3.455
3.738	3.736
4.089	4.089
4.392	4.391
4.654	4.668

Maximum Acceleration: 1017 g's