

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K10823 Temperature: 26.1 °C

Model: KICHER PR Humidity: 51%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

370.3 mv/5000g

(74.1 μ v/g)

R²: 0.999983 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 01Jul2026

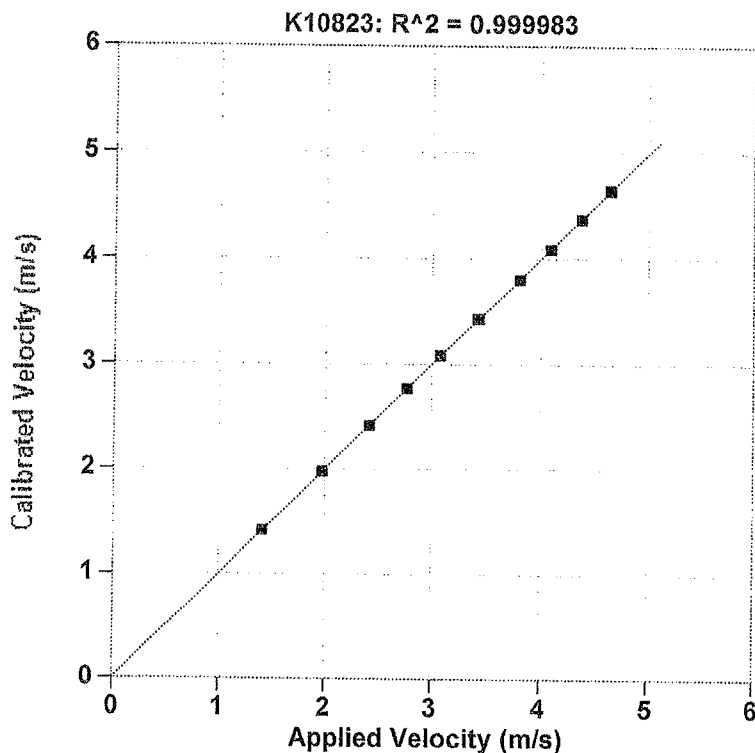

Reference Velocity	S/N K10823 Velocity
m/s	m/s
1.417	1.419
1.980	1.980
2.422	2.417
2.770	2.771
3.081	3.086
3.429	3.435
3.809	3.807
4.100	4.093
4.386	4.383
4.652	4.655
Maximum Acceleration: 1039 g's	