


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

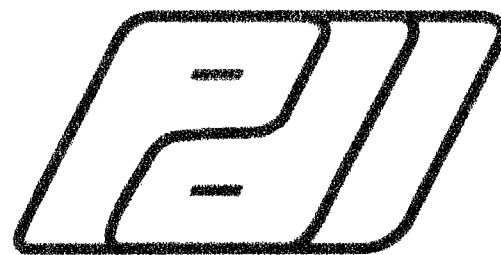

Serial No: K10824 Temperature: 23.6 °C

Model: KICHER PR Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

383.4 mv/5000g

(76.7 μ v/g)

R²: 0.999980 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 31Jul2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

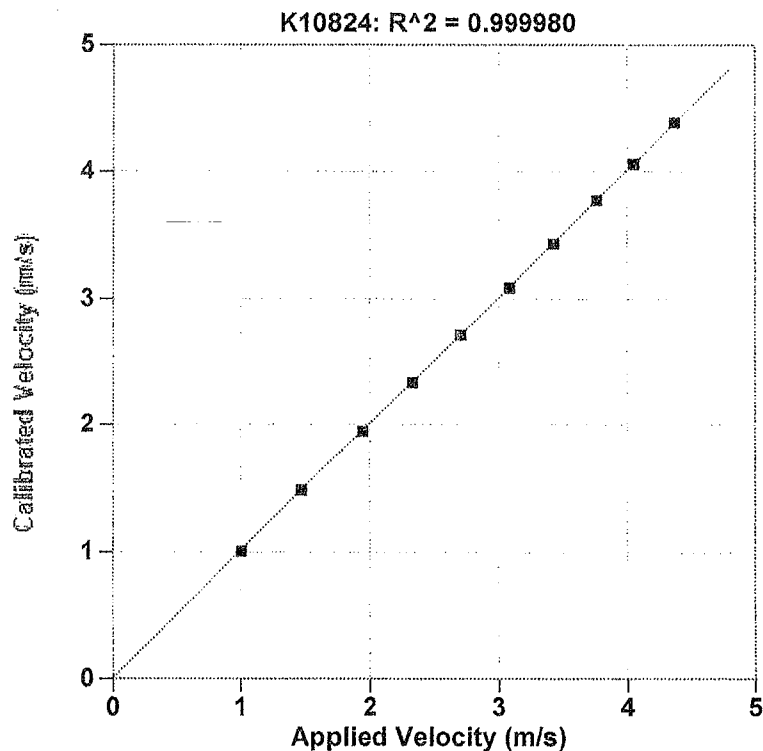

Reference Velocity	S/N K10824 Velocity
m/s	m/s
1.010	1.003
1.480	1.479
1.948	1.941
2.337	2.333
2.712	2.713
3.091	3.088
3.436	3.432
3.771	3.772
4.053	4.054
4.376	4.385

Maximum Acceleration: 949 g's