


# Certificate of Calibration

## Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

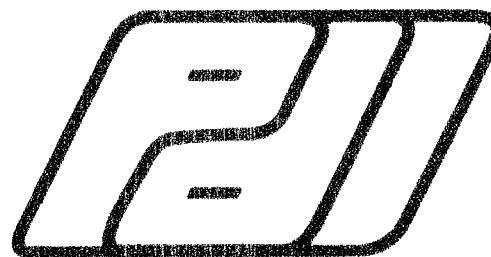

Serial No: K10990 Temperature: 23.8 °C

Model: KICHER PR Humidity: 66%

Calibrated on: Channel 3 on 8G 5161 LE

### PDA CALIBRATION FACTOR

420.7 mv/5000g


(84.1  $\mu$ v/g)

R<sup>2</sup>: 0.999988 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025  
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025  
958 g's/volt


Operator: William Johnson

  
Signed

Reference accelerometer calibrations are traceable to  
the United States National Institute of Standards and  
Technology (NIST).

Calibration valid 2 years

From: 09Jun2026

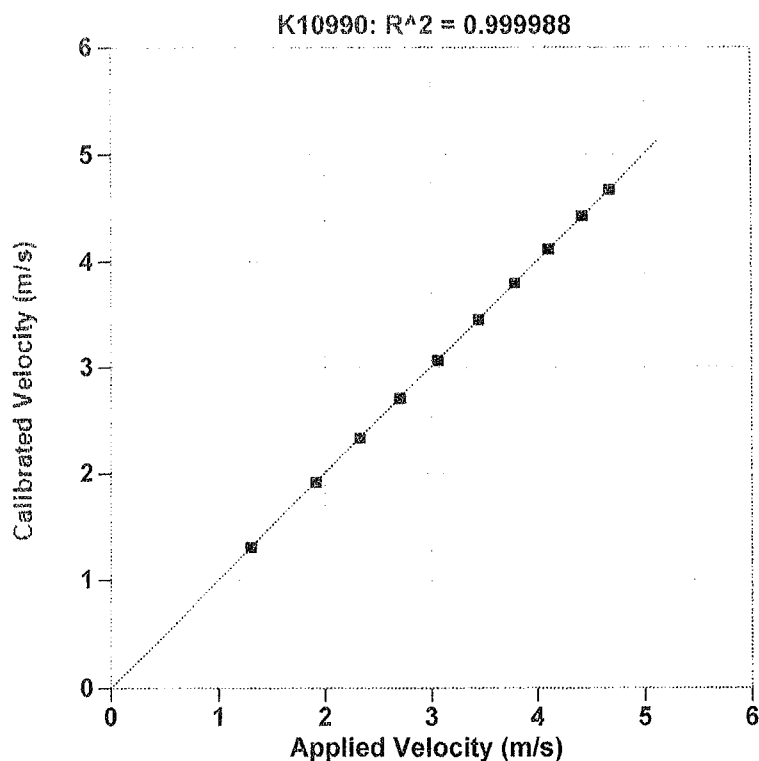

| Reference Velocity | S/N K10990 Velocity |
|--------------------|---------------------|
| m/s                | m/s                 |
| 1.311              | 1.306               |
| 1.918              | 1.918               |
| 2.333              | 2.331               |
| 2.711              | 2.704               |
| 3.067              | 3.064               |
| 3.451              | 3.449               |
| 3.796              | 3.798               |
| 4.113              | 4.116               |
| 4.422              | 4.427               |
| 4.678              | 4.679               |

Maximum Acceleration: 1018 g's