

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K11198 Temperature: 22.4 °C

Model: KICHER PR Humidity: 38%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

407.6 mv/5000g

(81.5 μ v/g)

R²: 0.999926 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 01Aug2026

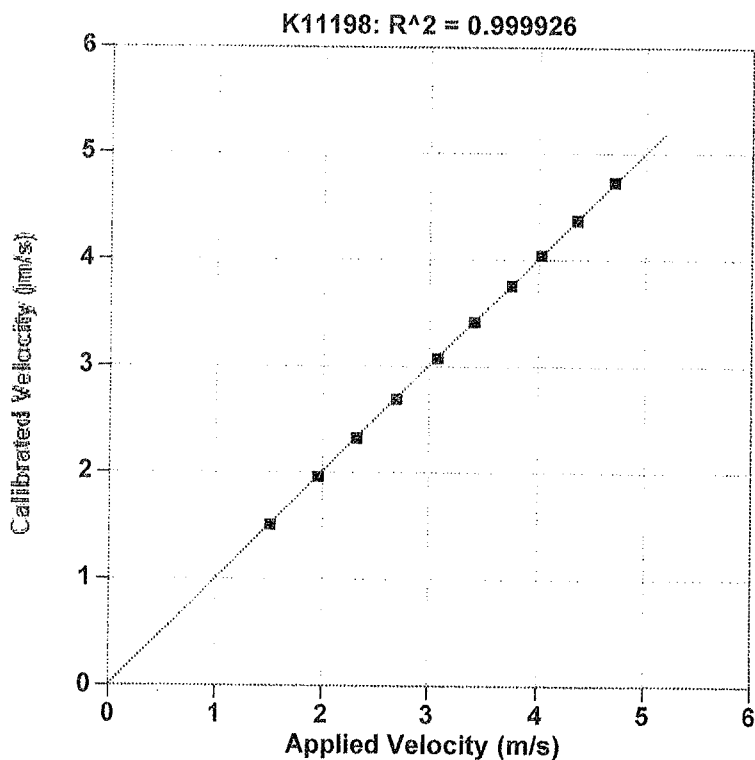

Reference Velocity	S/N K11198 Velocity
m/s	m/s
1.515	1.506
1.964	1.953
2.325	2.317
2.698	2.687
3.078	3.070
3.414	3.412
3.752	3.753
4.029	4.037
4.362	4.365
4.710	4.724

Maximum Acceleration: 1031 g's