

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K11392 Temperature: 23.1 °C

Model: KICHER PR Humidity: 40%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

389.6 mv/5000g

(77.9 μ v/g)

R²: 0.999990 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 05Aug2026

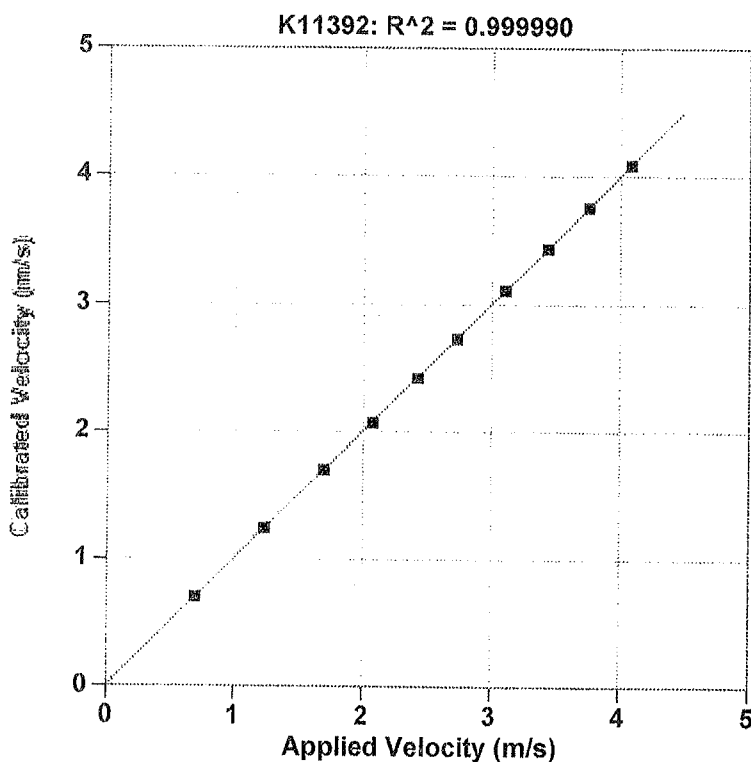

Reference Velocity	S/N K11392 Velocity
m/s	m/s
0.696	0.697
1.241	1.240
1.695	1.699
2.076	2.070
2.424	2.423
2.730	2.727
3.105	3.110
3.435	3.436
3.757	3.759
4.087	4.085

Maximum Acceleration: 881 g's