


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

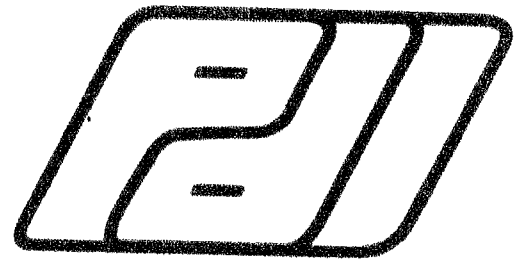

Serial No: K11403 Temperature: 22.9 °C

Model: KICHER PR Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

366.1 mv/5000g

(73.2 μ v/g)

R^2: 0.999993 [Chip programmed]


Operator: William Johnson

William Johnson

Signed

Calibration valid 2 years

From: 05Aug2026

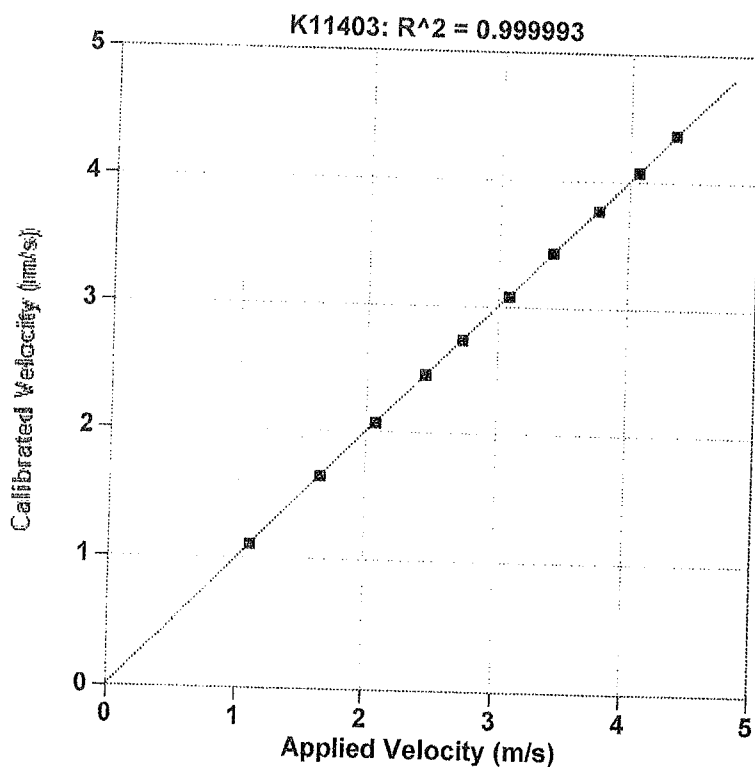

Reference Velocity	S/N K11403 Velocity
m/s	m/s
1.108	1.105
1.650	1.647
2.074	2.070
2.450	2.452
2.730	2.730
3.085	3.083
3.427	3.424
3.767	3.770
4.074	4.074
4.363	4.368

Maximum Acceleration: 949 g's