


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

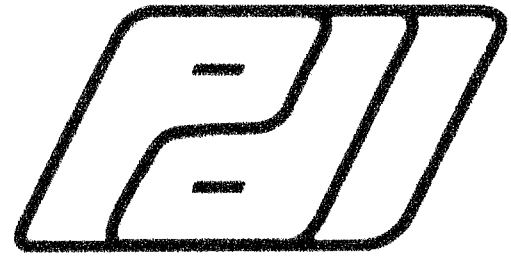

Serial No: K11961 Temperature: 26.1 °C

Model: KICHER PR Humidity: 51%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

441.2 mv/5000g


(88.2 μ v/g)

R²: 0.999945 [Chip programmed]

Ref Acc 1: 85363I Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382I Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Calibration valid 2 years

From: 01Jul2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

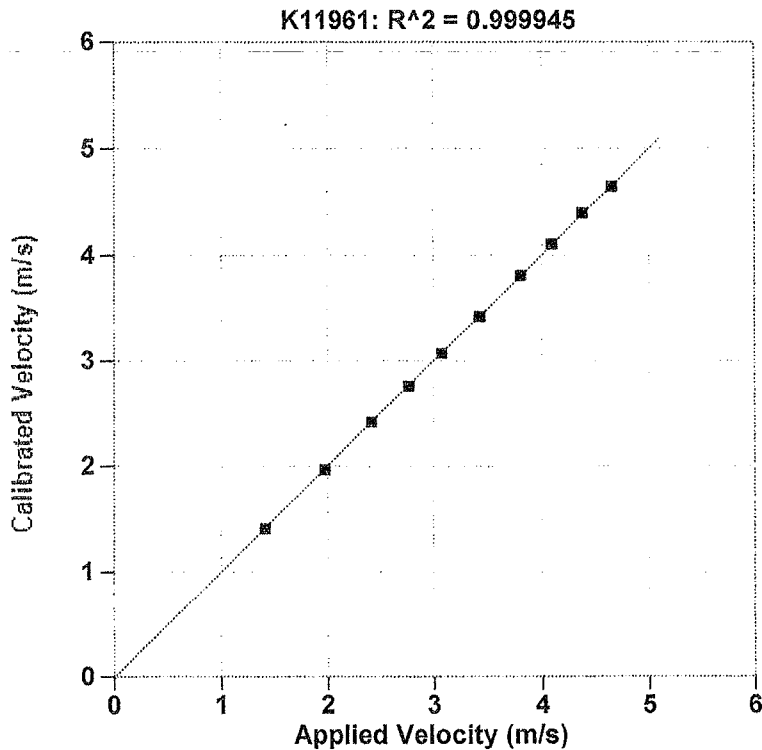

Reference Velocity	S/N K11961 Velocity
m/s	m/s
1.417	1.409
1.980	1.970
2.422	2.418
2.770	2.763
3.081	3.074
3.429	3.425
3.809	3.814
4.100	4.108
4.386	4.400
4.652	4.649
Maximum Acceleration: 1039 g's	