


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

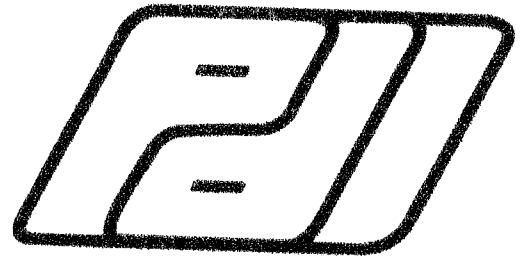

Serial No: K12177 Temperature: 23.3 °C
Model: KICHER PR Humidity: 41%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

388.0 mv/5000g
(77.6 μ v/g)
R²: 0.999948 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 05Aug2026

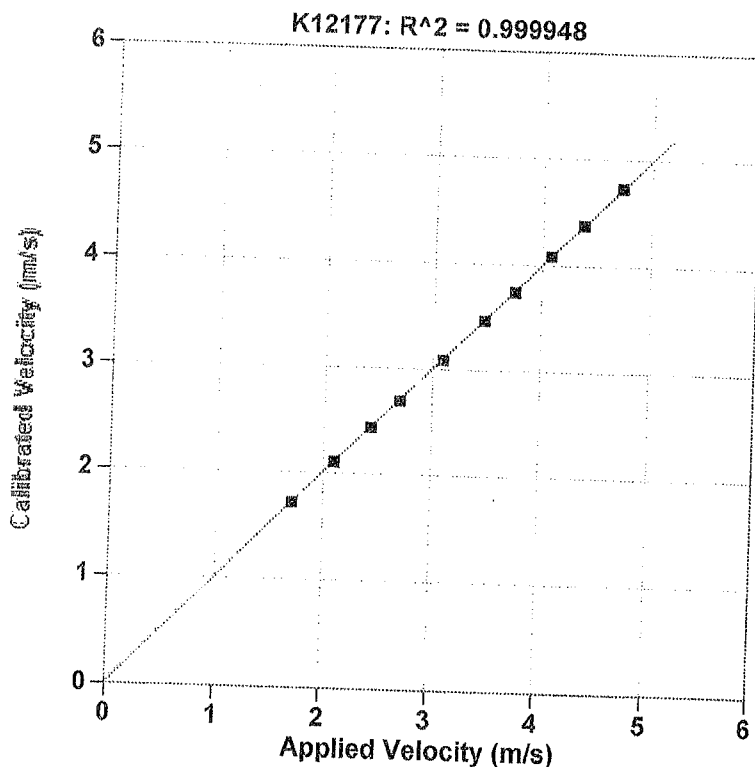

Reference Velocity	S/N K12177 Velocity
m/s	m/s
1.711	1.710
2.099	2.099
2.437	2.434
2.703	2.691
3.094	3.086
3.474	3.468
3.752	3.745
4.084	4.088
4.374	4.383
4.729	4.739

Maximum Acceleration: 1030 g's