


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

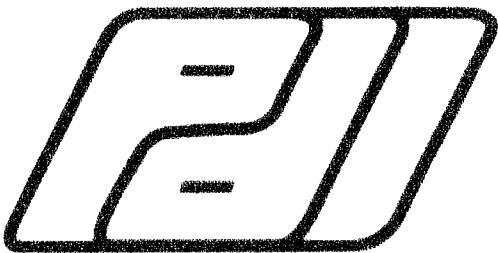

Serial No: K12178 Temperature: 23.3 °C
Model: KICHER PR Humidity: 40%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

414.7 mv/5000g
(82.9 µv/g)
R^2: 0.999969 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Will Johnson
Signed

Calibration valid 2 years

From: 05Aug2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

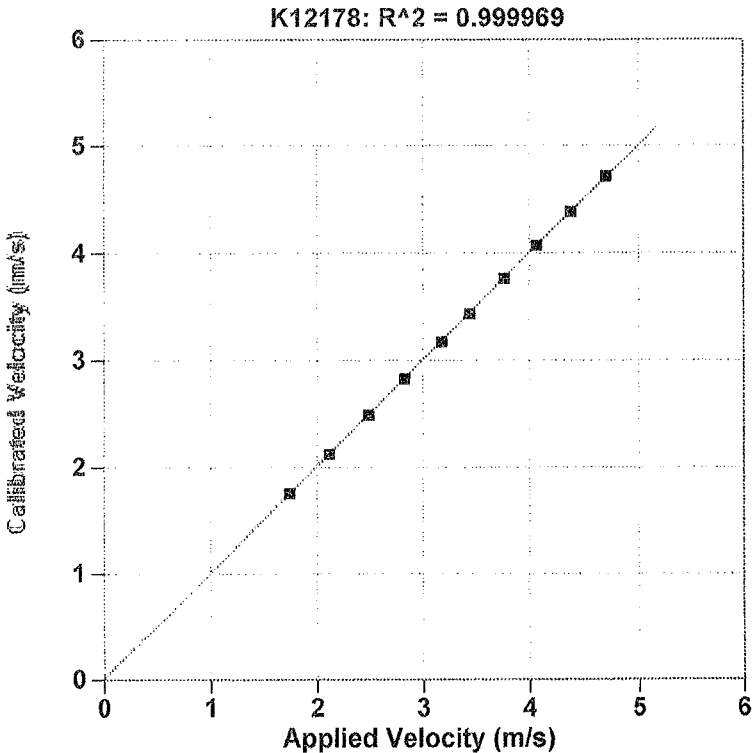

Reference Velocity	S/N K12178 Velocity
m/s	m/s
1.747	1.751
2.116	2.121
2.487	2.487
2.826	2.823
3.175	3.170
3.439	3.433
3.768	3.762
4.071	4.068
4.382	4.389
4.709	4.717
Maximum Acceleration: 1029 g's	