

Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12179 Temperature: 23.3 °C
Model: KICHER PR Humidity: 41%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

391.4 mv/5000g
(78.3 μ v/g)
 R^2 : 0.999951 [Chip programmed]


Operator: William Johnson

[Signature]
Signed

Calibration valid 2 years

From: 05Aug2026

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

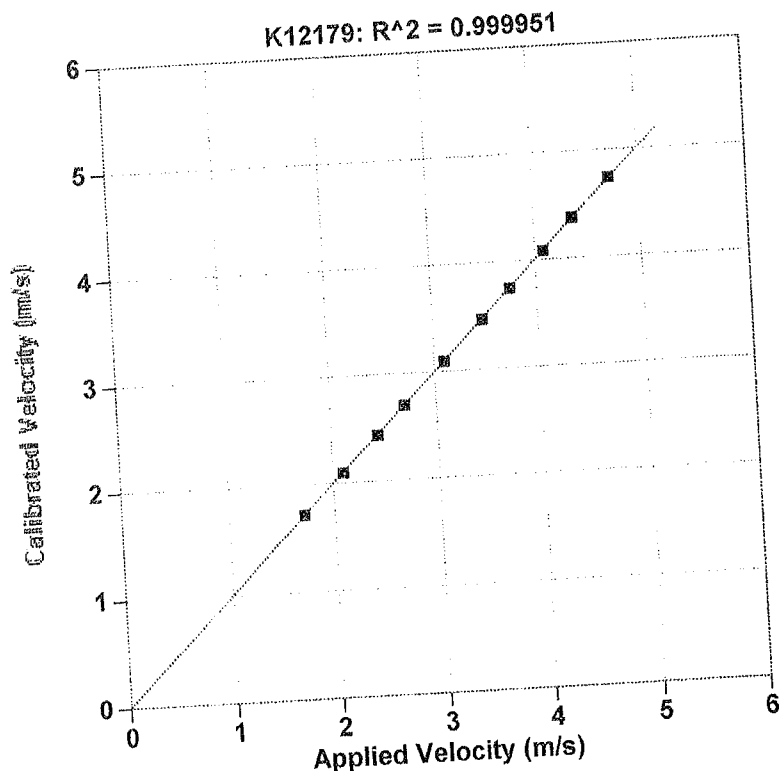

Reference Velocity	S/N K12179 Velocity
m/s	m/s
1.711	1.715
2.099	2.092
2.437	2.428
2.703	2.703
3.094	3.094
3.474	3.465
3.752	3.747
4.084	4.081
4.374	4.380
4.729	4.742
Maximum Acceleration: 1030 g's	