


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

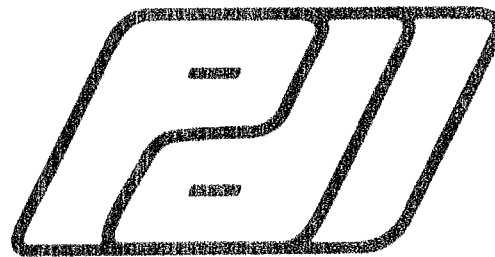

Serial No: K1242 Temperature: 24.0 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

322.1 mv/5000g


(64.4 μ v/g)

R²: 0.999975 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Calibration valid 2 years

From: 10Aug2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

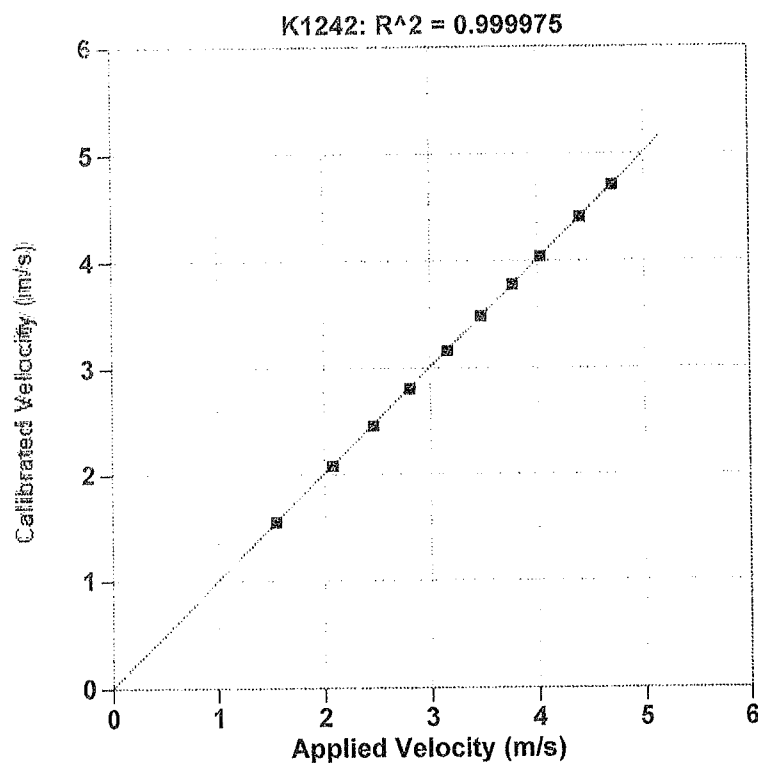

Reference Velocity	S/N K1242 Velocity
m/s	m/s
1.547	1.549
2.081	2.078
2.463	2.454
2.811	2.804
3.160	3.156
3.476	3.484
3.772	3.777
4.036	4.035
4.400	4.403
4.707	4.707

Maximum Acceleration: 1037 g's