


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

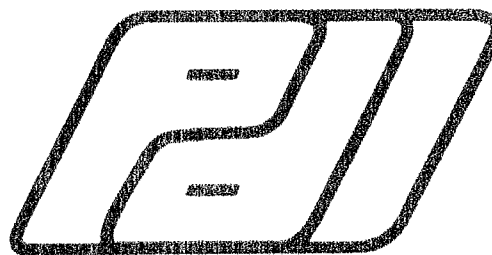

Serial No: K1266 Temperature: 24.0 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

330.7 mv/5000g

(66.1 μ v/g)

R²: 0.999985 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 10Aug2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

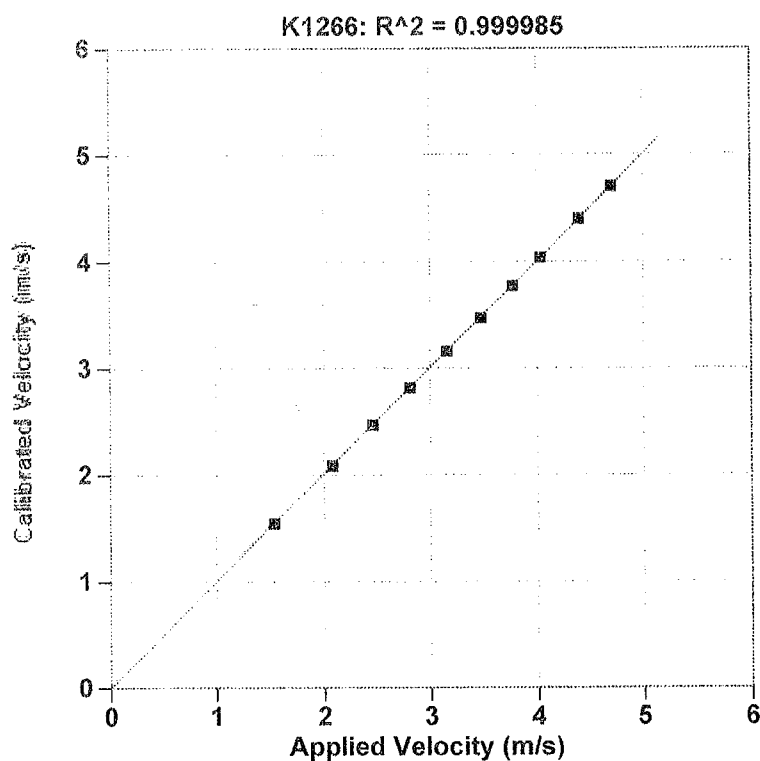

Reference Velocity	S/N K1266 Velocity
m/s	m/s
1.547	1.542
2.081	2.079
2.463	2.460
2.811	2.811
3.160	3.156
3.476	3.471
3.772	3.771
4.036	4.039
4.400	4.406
4.707	4.710

Maximum Acceleration: 1037 g's