

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K12796 Temperature: 21.0 °C

Model: KICHER PR Humidity: 49%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

369.2 mv/5000g

(73.8 μ v/g)

R²: 0.999982 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 20Aug2026

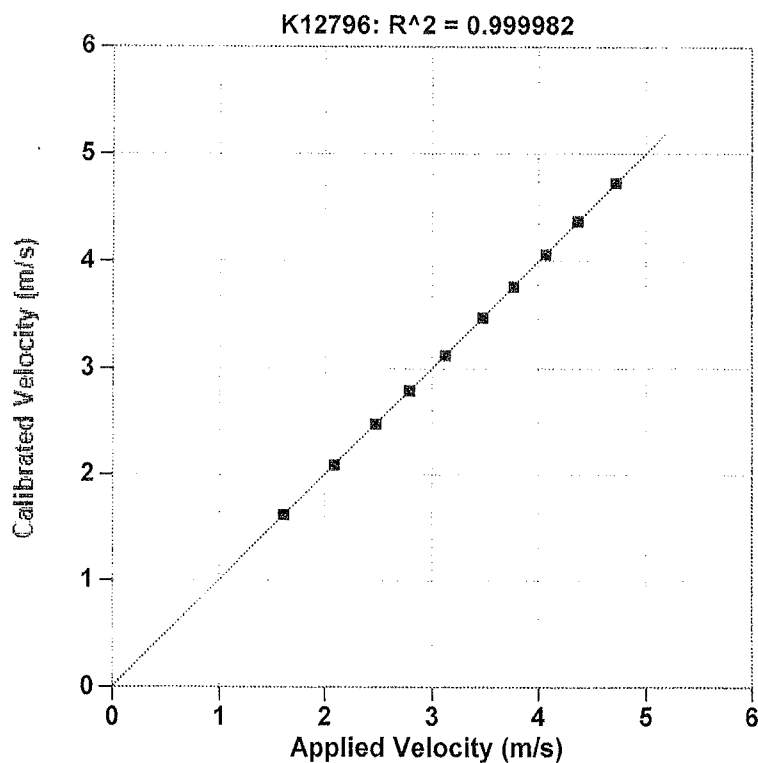

Reference Velocity	S/N K12796 Velocity
m/s	m/s
1.608	1.611
2.091	2.087
2.472	2.469
2.785	2.789
3.119	3.120
3.474	3.474
3.766	3.761
4.071	4.065
4.371	4.375
4.726	4.732

Maximum Acceleration: 1019 g's