

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.




Serial No: K12938 Temperature: 22.4 °C
Model: KICHER PR Humidity: 38%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

397.8 mv/5000g
(79.6 μv/g)
R^2: 0.999963 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 01Aug2026

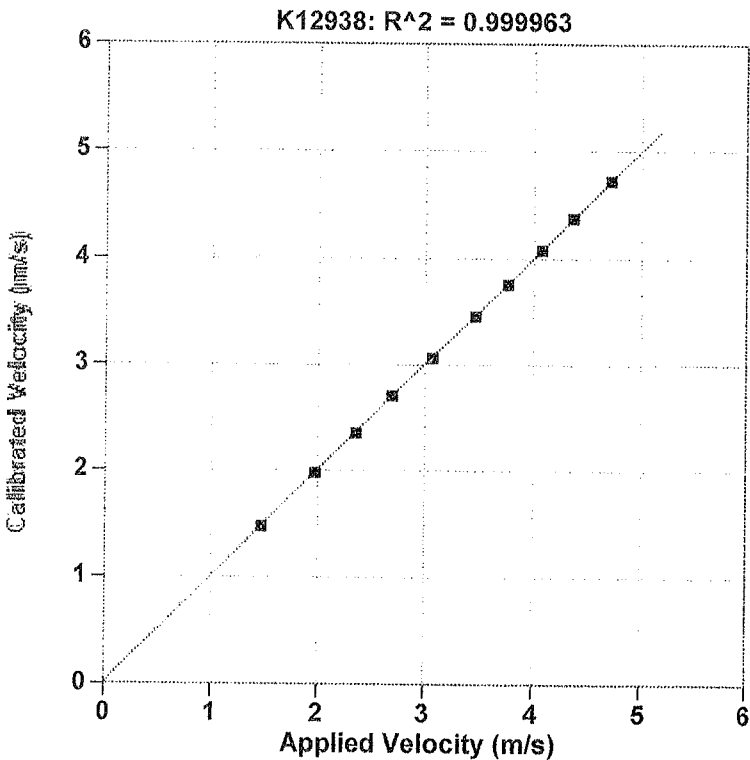

Reference Velocity	S/N K12938 Velocity
m/s	m/s
1.469	1.466
1.979	1.972
2.360	2.351
2.699	2.700
3.067	3.058
3.460	3.459
3.760	3.757
4.075	4.078
4.367	4.378
4.725	4.729
Maximum Acceleration: 1034 g's	