


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

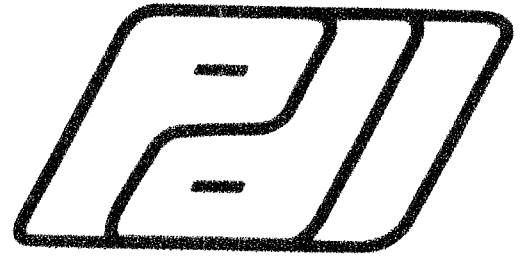

Serial No: K13193 Temperature: 23.1 °C

Model: KICHER PR Humidity: 40%

Calibrated on: Channel 3 on 8G 5161 LE

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

PDA CALIBRATION FACTOR

393.5 mv/5000g

(78.7 μ v/g)


R^2: 0.999974 [Chip programmed]

Operator: William Johnson

William Johnson
Signed

Calibration valid 2 years

From: 05Aug2026

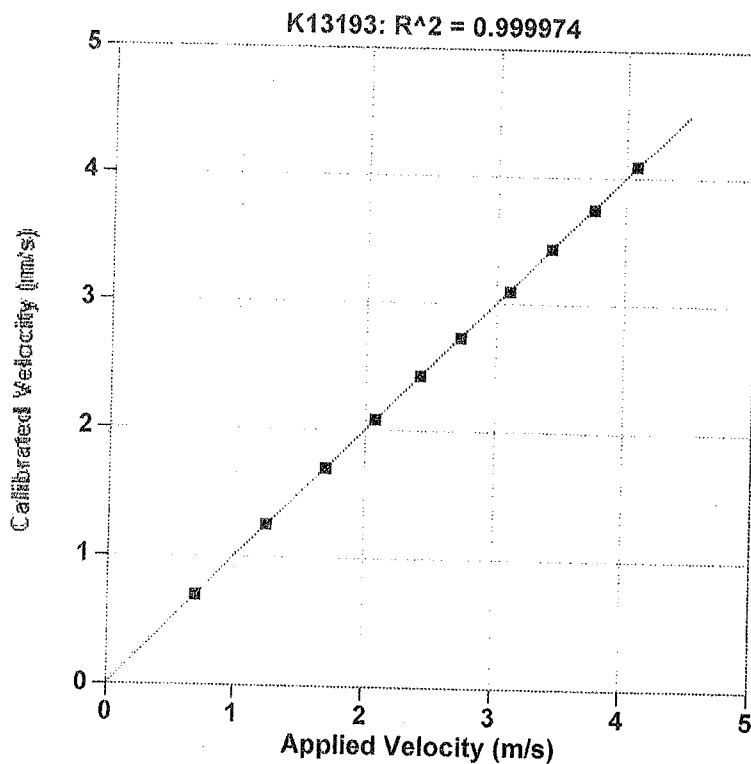

Reference Velocity	S/N K13193 Velocity
m/s	m/s
0.696	0.697
1.241	1.249
1.695	1.697
2.076	2.083
2.424	2.427
2.730	2.728
3.105	3.097
3.435	3.435
3.757	3.749
4.087	4.093
Maximum Acceleration: 881 g's	