

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15435 Temperature: 23.3 °C

Model: KICHER PR Humidity: 39%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

395.6 mv/5000g

(79.1 μ v/g)

R²: 0.999921 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson




Signed

Calibration valid 2 years

From: **AUG 17 2026**

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

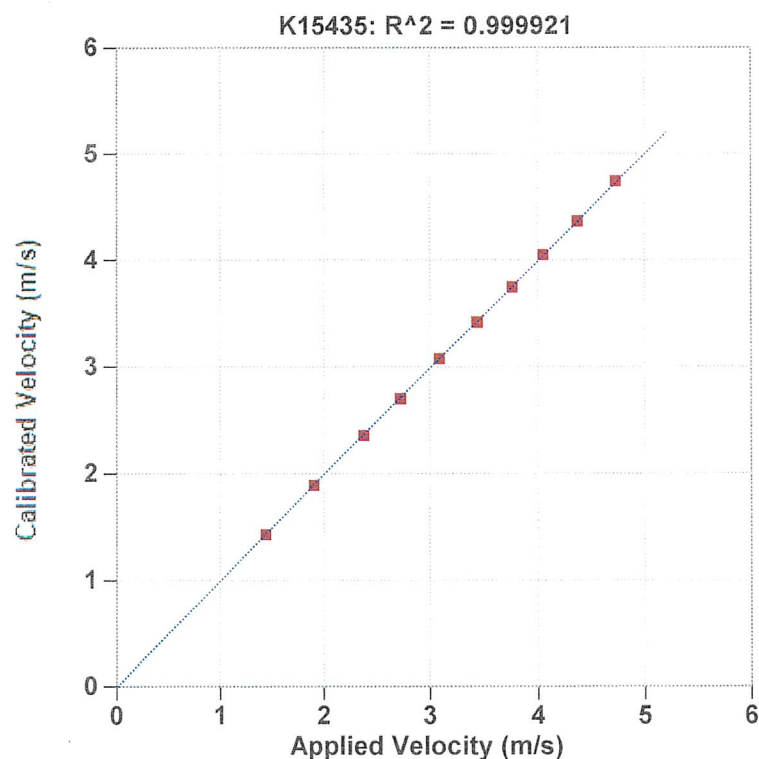

Reference Velocity	S/N K15435 Velocity
m/s	m/s
1.435	1.431
1.900	1.894
2.375	2.362
2.721	2.708
3.085	3.082
3.432	3.424
3.757	3.753
4.045	4.055
4.369	4.373
4.731	4.747

Maximum Acceleration: 1037 g's