

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15436 Temperature: 23.3 °C
Model: KICHER PR Humidity: 39%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

427.8 mv/5000g
(85.6 μv/g)
R^2: 0.999929 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: **AUG 17 2026**

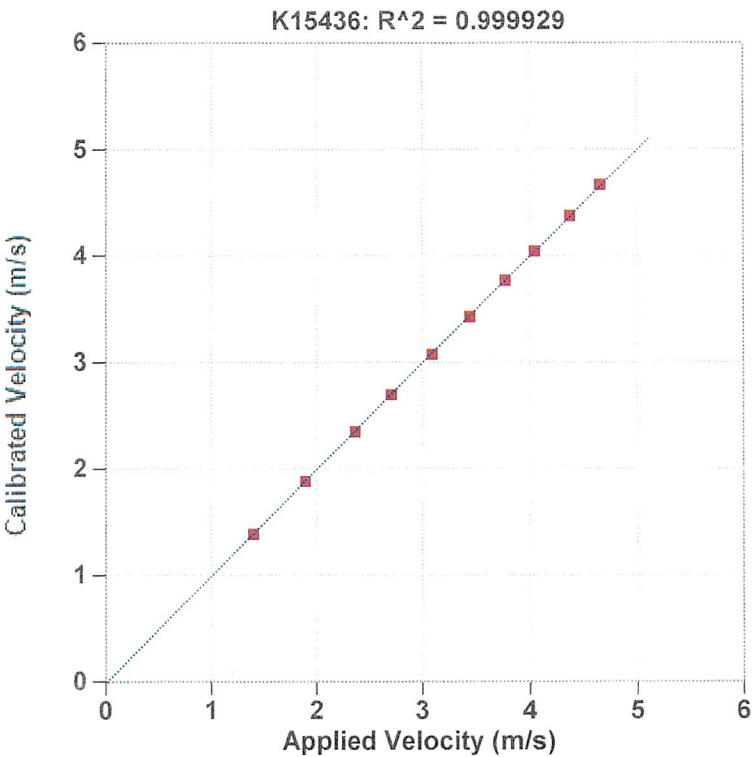

Reference Velocity	S/N K15436 Velocity
m/s	m/s
1.392	1.385
1.890	1.884
2.357	2.349
2.703	2.697
3.087	3.077
3.440	3.430
3.773	3.769
4.039	4.045
4.368	4.376
4.653	4.670

Maximum Acceleration: 1014 g's