

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15439 Temperature: 23.3 °C

Model: KICHER PR Humidity: 39%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

396.1 mv/5000g

(79.2 μ v/g)

R²: 0.999965 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson


Signed

Calibration valid 2 years

AUG 17 2026

From: _____

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

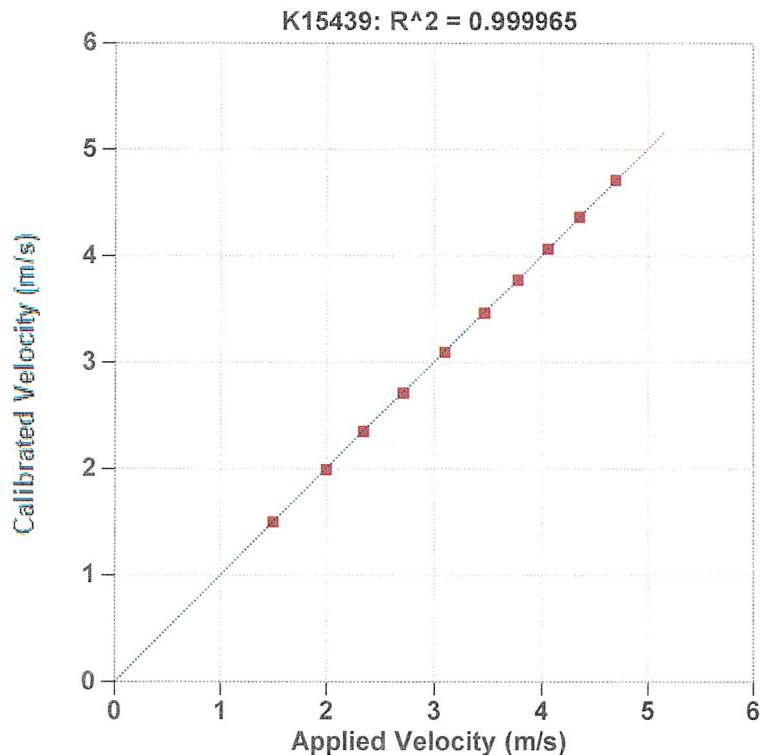

Reference Velocity	S/N K15439 Velocity
m/s	m/s
1.499	1.499
2.001	1.990
2.353	2.346
2.714	2.710
3.099	3.095
3.471	3.464
3.770	3.773
4.061	4.064
4.361	4.365
4.701	4.710

Maximum Acceleration: 1024 g's