

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15460 Temperature: 23.8 °C

Model: KICHER PR Humidity: 45%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

373.6 mv/5000g


(74.7 μ v/g)

R²: 0.999937 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson




Signed

Calibration valid 2 years

From: AUG 14 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

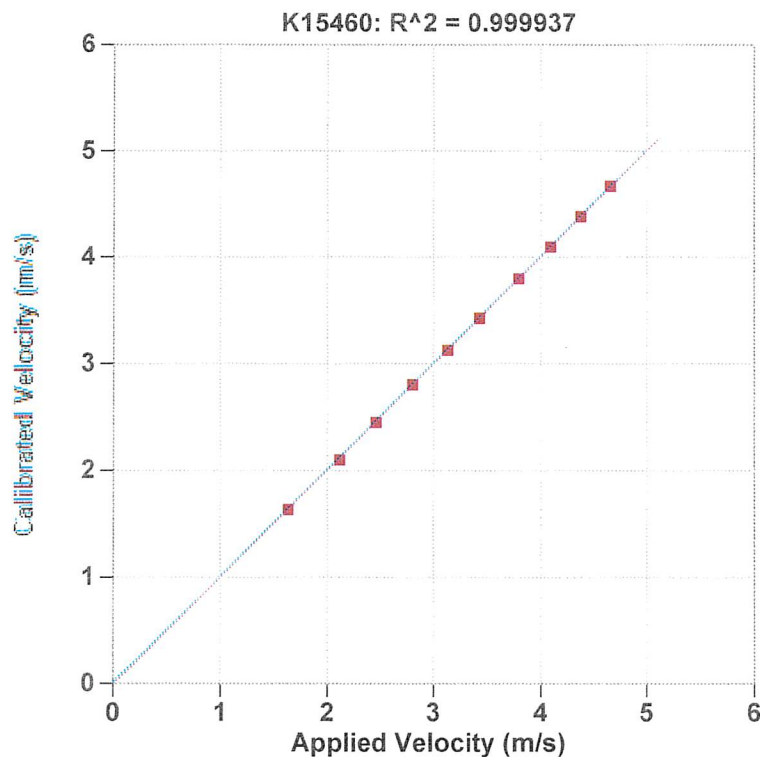

Reference Velocity	S/N K15460 Velocity
m/s	m/s
1.641	1.632
2.116	2.102
2.463	2.451
2.807	2.806
3.132	3.131
3.431	3.432
3.799	3.799
4.093	4.097
4.380	4.382
4.658	4.669
Maximum Acceleration: 1018 g's	