


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

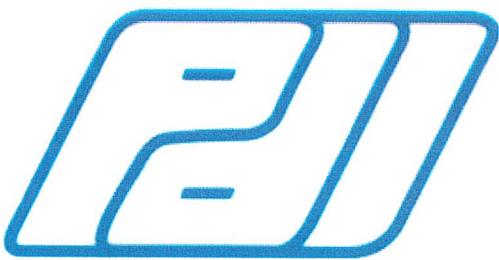

Serial No: K15469 Temperature: 20.7 °C
Model: KICHER PR Humidity: 45%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

411.1 mv/5000g
(82.2 μv/g)
R^2: 0.999957 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: **AUG 27 2026**

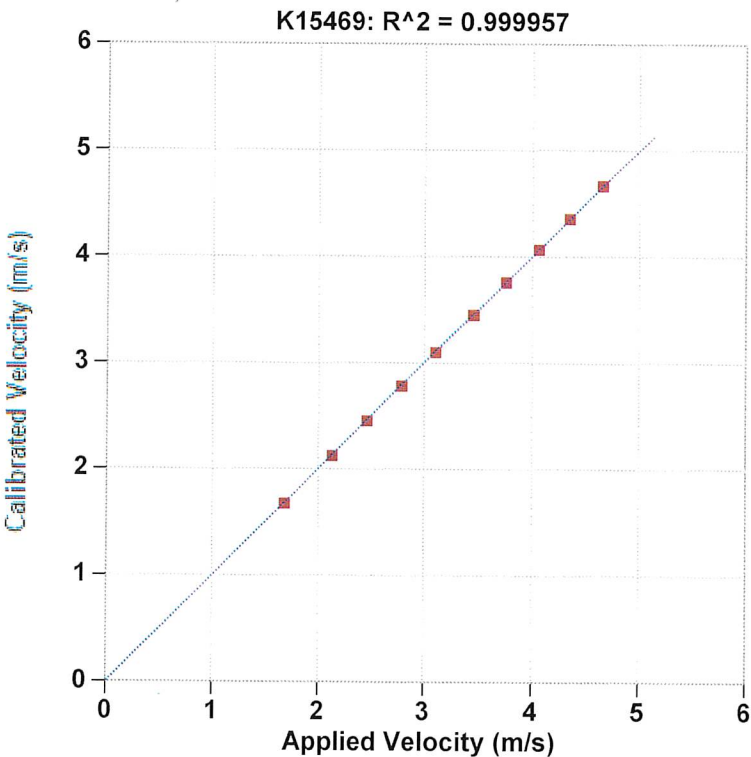

Reference Velocity	S/N K15469 Velocity
m/s	m/s
1.676	1.672
2.130	2.121
2.459	2.450
2.786	2.779
3.104	3.099
3.451	3.449
3.751	3.756
4.057	4.064
4.348	4.353
4.662	4.666

Maximum Acceleration: 1012 g's