

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15492 Temperature: 19.9 °C
Model: KICHER PR Humidity: 48%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

401.7 mv/5000g
(80.3 μv/g)
R^2: 0.999962 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: AUG 26 2026

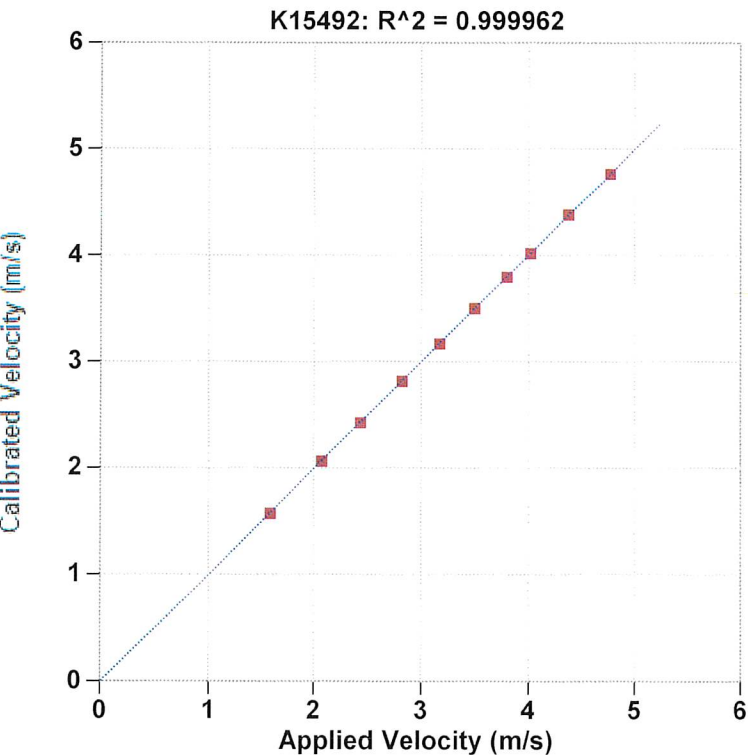

Reference Velocity	S/N K15492 Velocity
m/s	m/s
1.583	1.573
2.073	2.066
2.431	2.425
2.819	2.814
3.170	3.166
3.496	3.500
3.796	3.793
4.017	4.018
4.376	4.384
4.757	4.764
Maximum Acceleration: 1052 g's	