

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15493 Temperature: 19.9 °C
Model: KICHER PR Humidity: 50%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

428.0 mv/5000g
(85.6 μv/g)
R^2: 0.999911 [Chip programmed]


Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years
AUG 27 2026
From: _____

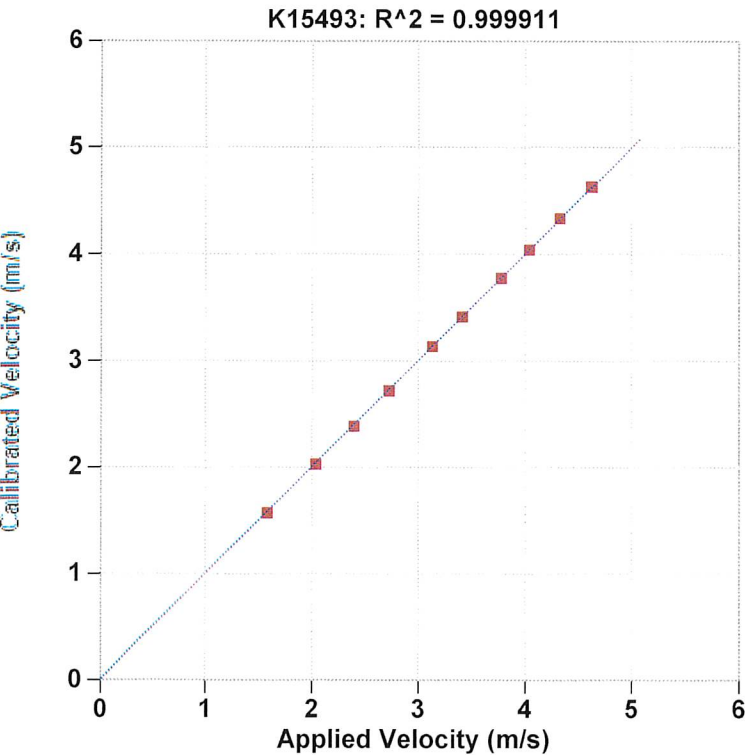

Reference Velocity	S/N K15493 Velocity
m/s	m/s
1.574	1.564
2.036	2.023
2.395	2.379
2.723	2.715
3.130	3.129
3.412	3.410
3.777	3.774
4.036	4.041
4.326	4.335
4.622	4.634
Maximum Acceleration: 1020 g's	