

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15496 Temperature: 19.9 °C
Model: KICHER PR Humidity: 50%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

393.3 mv/5000g
(78.7 μv/g)
R^2: 0.999905 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson




Signed

Calibration valid 2 years

From: AUG 27 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

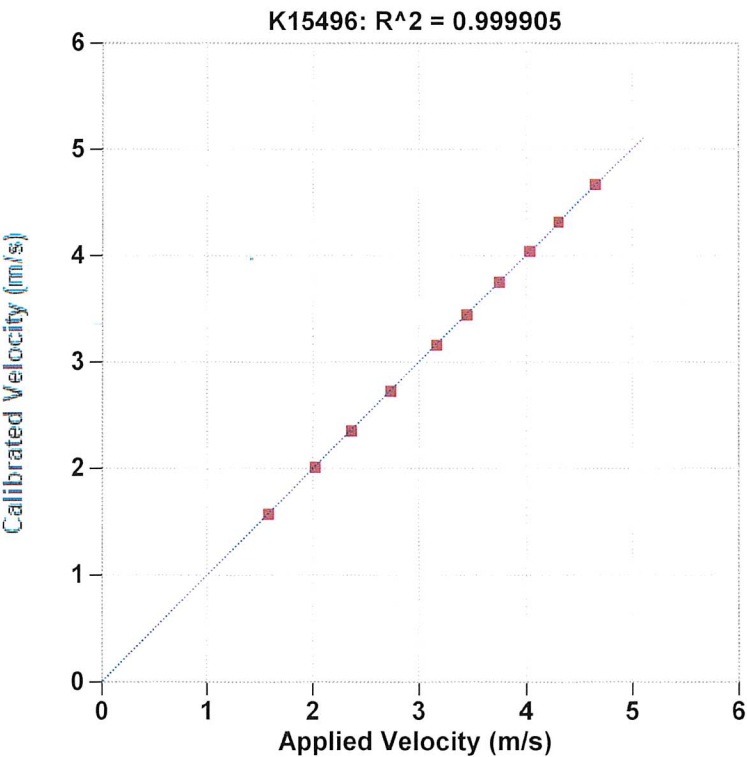

Reference Velocity	S/N K15496 Velocity
m/s	m/s
1.573	1.567
2.019	2.008
2.361	2.349
2.731	2.723
3.164	3.154
3.447	3.439
3.748	3.747
4.029	4.038
4.301	4.312
4.653	4.666

Maximum Acceleration: 1032 g's