

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15498 Temperature: 19.9 °C

Model: KICHER PR Humidity: 48%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

386.1 mv/5000g

(77.2 μ v/g)

R²: 0.999907 [Chip programmed]

Operator: William Johnson

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt


Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Signed

Calibration valid 2 years

From: **AUG 26 2026**

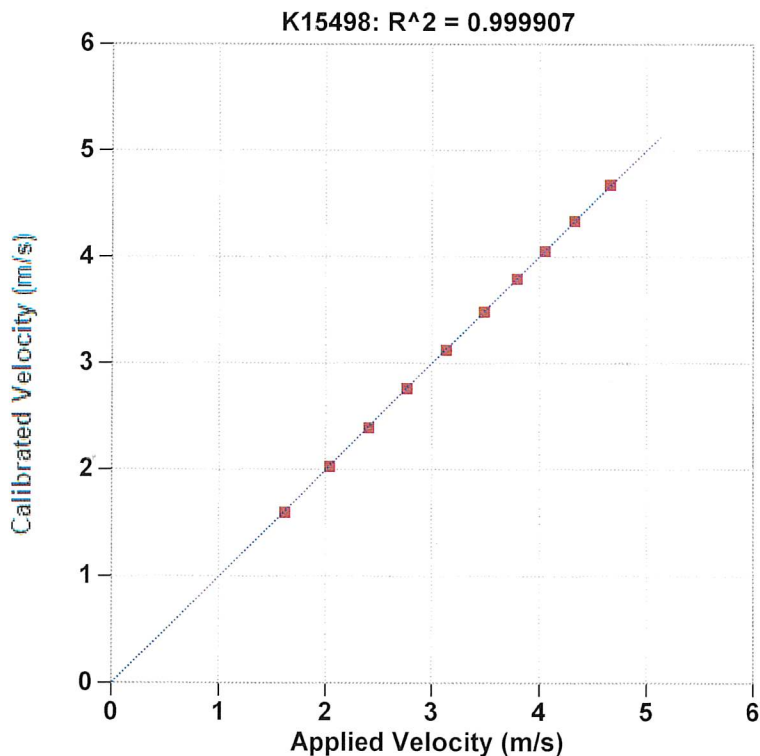

Reference Velocity	S/N K15498 Velocity
m/s	m/s
1.610	1.598
2.037	2.029
2.407	2.393
2.768	2.760
3.128	3.120
3.483	3.482
3.790	3.790
4.050	4.053
4.327	4.334
4.663	4.678

Maximum Acceleration: 1030 g's