

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15499 Temperature: 19.9 °C
Model: KICHER PR Humidity: 50%
Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

370.6 mv/5000g
(74.1 μv/g)
R^2: 0.999908 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Operator: William Johnson


Signed

Calibration valid 2 years

From: AUG 27 2026

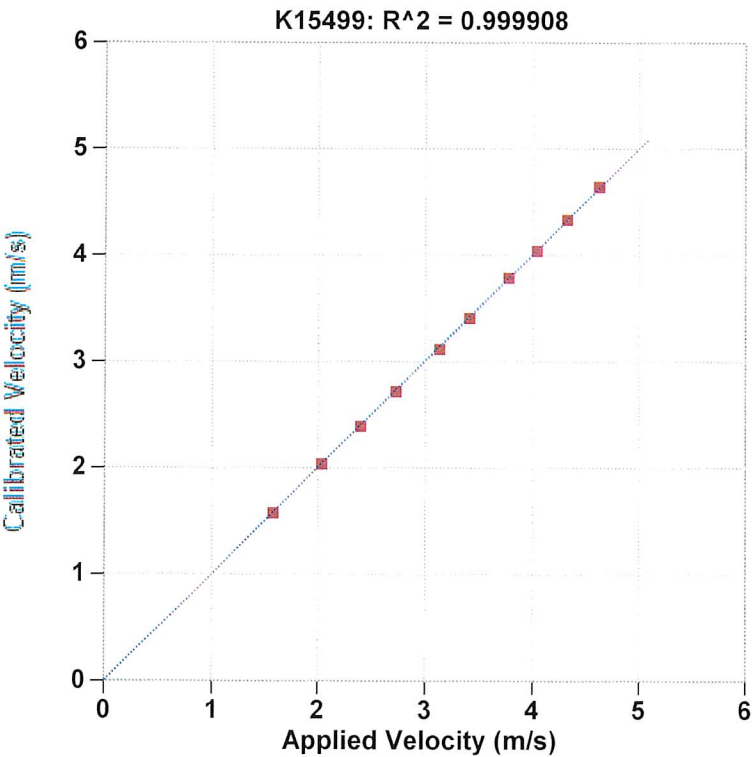

Reference Velocity	S/N K15499 Velocity
m/s	m/s
1.574	1.570
2.036	2.032
2.395	2.387
2.723	2.714
3.130	3.113
3.412	3.403
3.777	3.785
4.036	4.039
4.326	4.329
4.622	4.639

Maximum Acceleration: 1020 g's