

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15503 Temperature: 19.4 °C
Model: KICHER PR Humidity: 54%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

403.9 mv/5000g
(80.8 μv/g)
R^2: 0.999922 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: AUG 27 2026

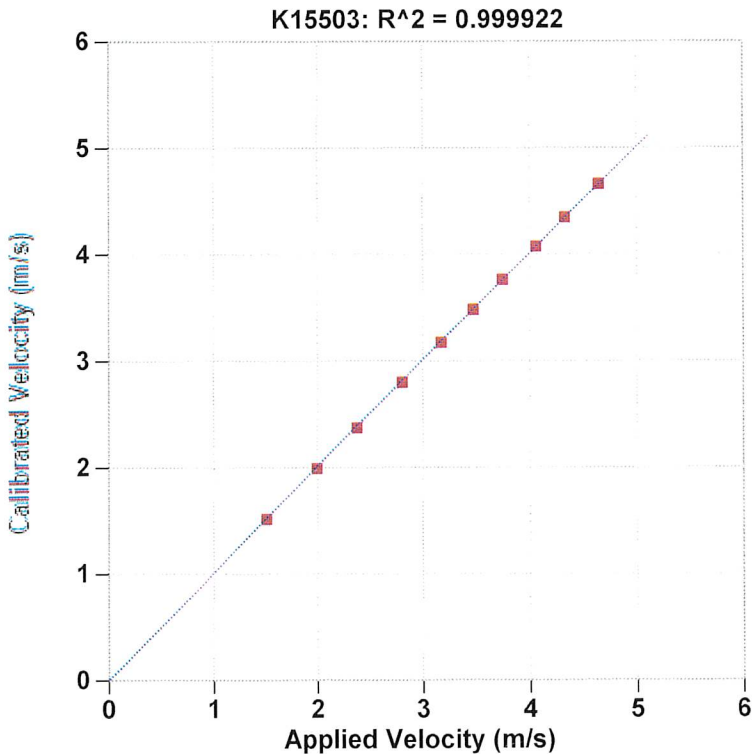

Reference Velocity	S/N K15503 Velocity
m/s	m/s
1.509	1.504
1.994	1.979
2.376	2.364
2.800	2.790
3.171	3.165
3.472	3.472
3.747	3.754
4.058	4.064
4.331	4.338
4.644	4.652

Maximum Acceleration: 1027 g's