

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15505 Temperature: 19.6 °C
Model: KICHER PR Humidity: 52%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

382.0 mv/5000g
(76.4 μv/g)
R^2: 0.999901 [Chip programmed]


Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt

Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years
From: **AUG 27 2026**

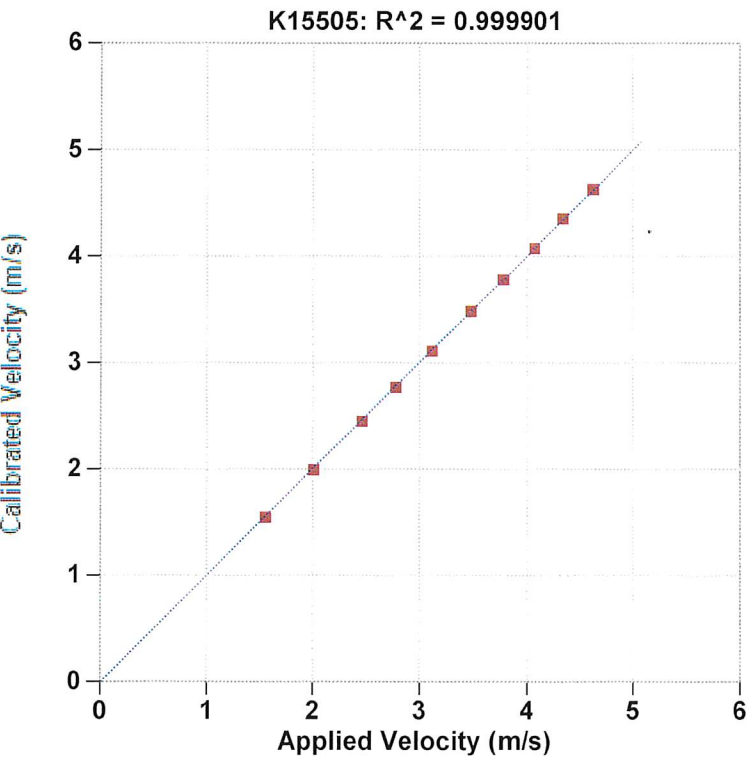

Reference Velocity	S/N K15505 Velocity
m/s	m/s
1.555	1.543
2.007	1.992
2.458	2.445
2.776	2.768
3.116	3.110
3.480	3.482
3.776	3.779
4.071	4.071
4.341	4.352
4.614	4.627
Maximum Acceleration: 1018 g's	