

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15509 Temperature: 19.3 °C
Model: KICHER PR Humidity: 53%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

418.5 mv/5000g
(83.7 μv/g)
R^2: 0.999938 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt
Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: AUG 27 2026

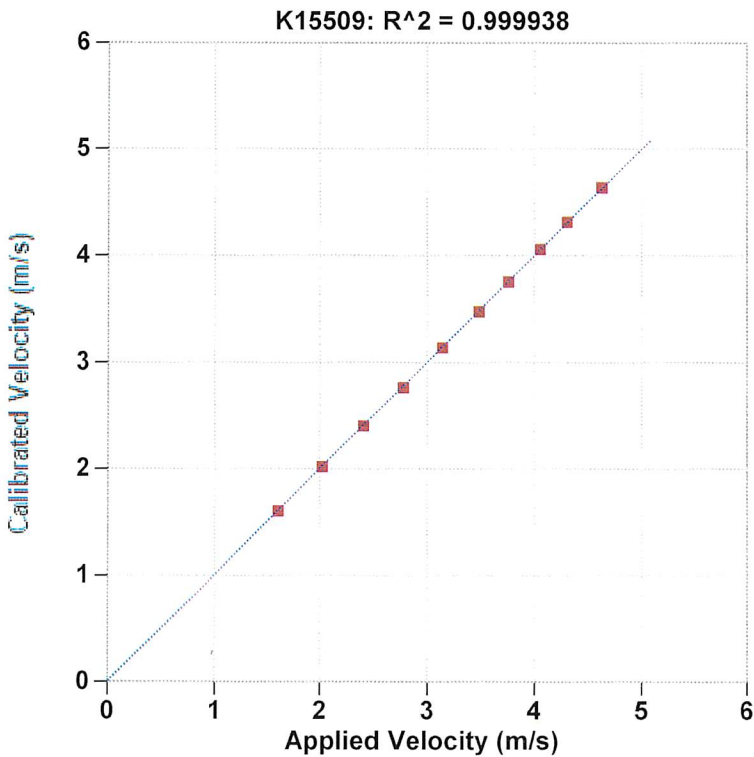

Reference Velocity	S/N K15509 Velocity
m/s	m/s
1.603	1.599
2.023	2.017
2.409	2.401
2.772	2.761
3.142	3.136
3.483	3.476
3.761	3.757
4.054	4.061
4.311	4.319
4.631	4.642

Maximum Acceleration: 1021 g's