




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 102A
PDI Gage Factor: 94.0
Mean Linear Correlation Coefficient: 0.999983

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-2532.8	-7.639	137.8	0.577
-2007.9	-5.995	662.7	2.162
-1469.8	-4.338	1148.3	3.674
-925.2	-2.699	1620.7	5.149
-393.7	-1.063	2014.4	6.380

Calibration Curve

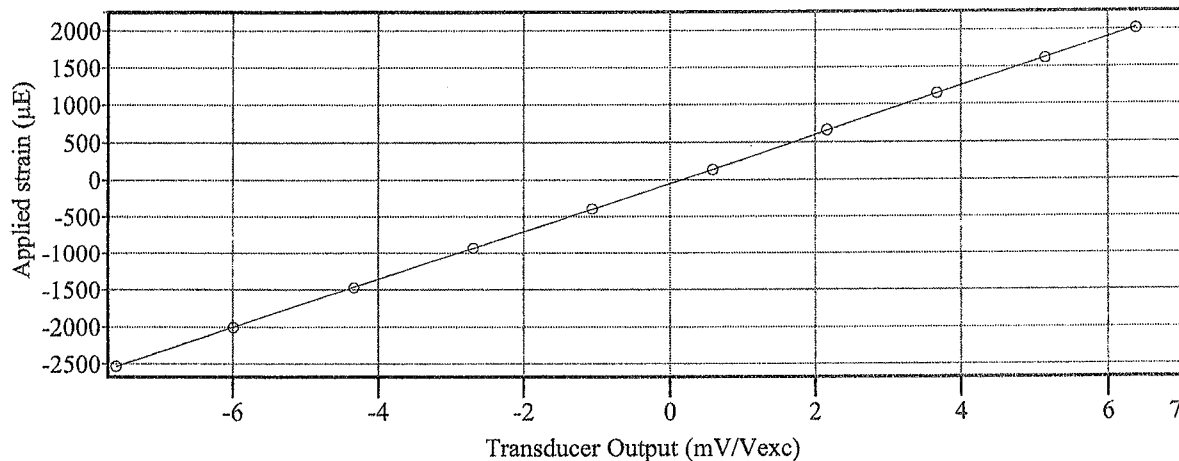

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: 102A

Calibration Date: 9/8/2026 7:46:24 AM

Calibration valid 2 years

