




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 107A
PDI Gage Factor: 92.6
Mean Linear Correlation Coefficient: 0.999779

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1857.0	-5.927	459.3	1.411
-1358.3	-4.377	833.3	2.548
-918.6	-3.008	1213.9	3.701
-520.6	-1.715	1581.4	4.824
-177.2	-0.573	2007.9	6.056
144.4	0.386		

Calibration Curve

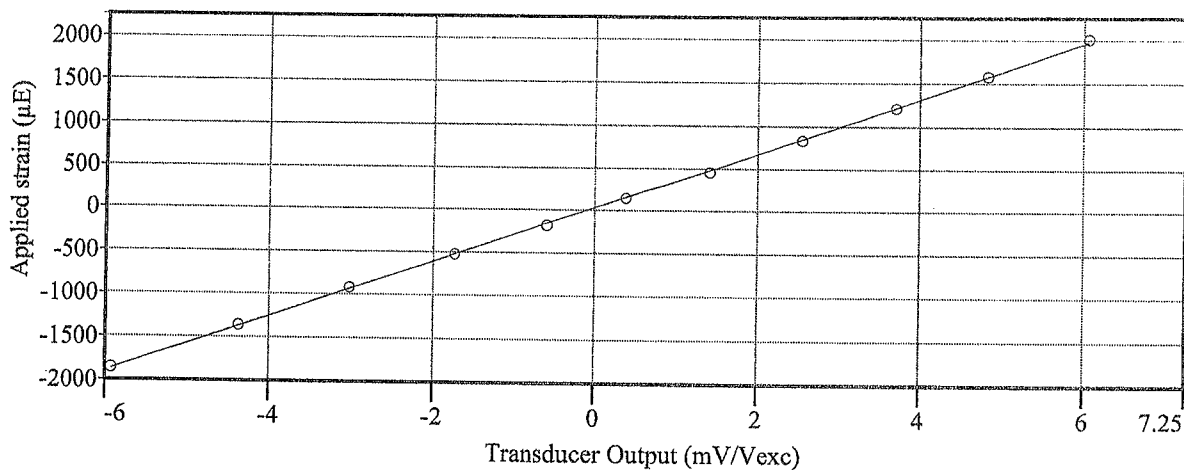

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature:

Paul Hartman

PDI Gage: 107A

Calibration Date: 9/8/2026 7:33:14 AM

Calibration valid 2 years

