


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

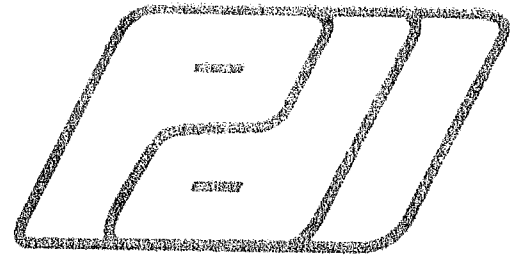

Serial No: 17670 Temperature: 21.1 °C

Model: PIT ACC Humidity: 49%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR


19.7 g's/volt

R²: 0.999948 [Chip programmed]

Ref Acc 1: LW547723! Cal on: 21Oct2025
10 g's/volt

Ref Acc 2: LW547722! Cal on: 21Oct2025
10 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: 17Aug2026

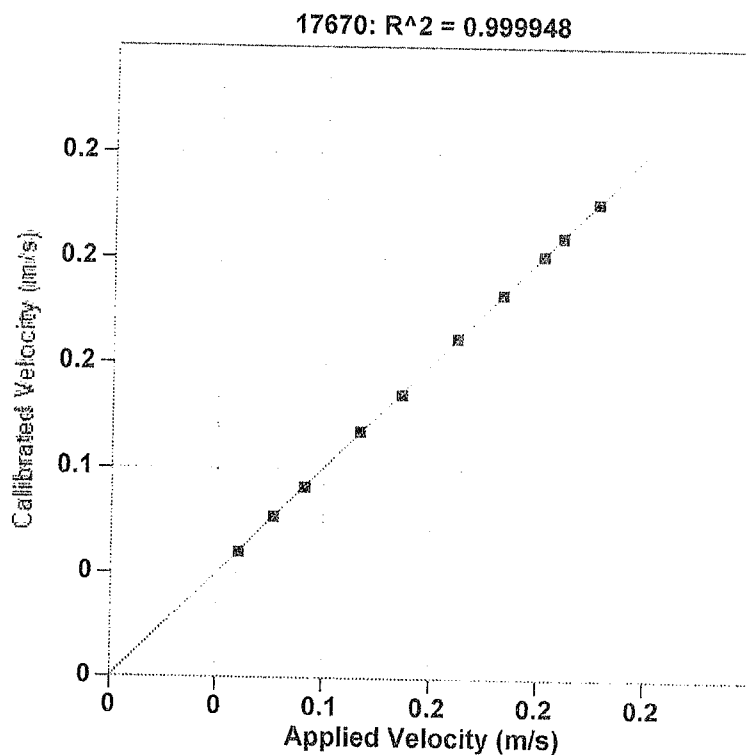

Reference Velocity	S/N 17670 Velocity
m/s	m/s
0.060	0.060
0.077	0.077
0.091	0.091
0.117	0.118
0.136	0.135
0.162	0.162
0.183	0.183
0.202	0.202
0.211	0.211
0.227	0.227
Maximum Acceleration: 27 g's	