




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 297A
PDI Gage Factor: 96.0
Mean Linear Correlation Coefficient: 0.999937

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1981.6	-6.001	498.7	1.500
-1528.9	-4.557	846.5	2.543
-1049.9	-3.110	1209.5	3.667
-590.6	-1.738	1581.4	4.790
-137.8	-0.454	2001.3	6.031
190.3	0.568		

Calibration Curve

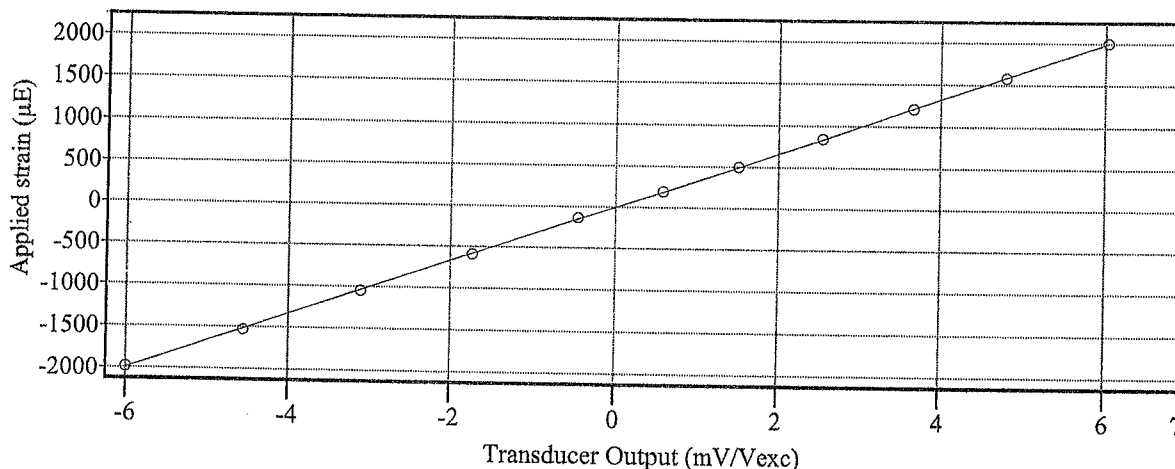

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

Signature: _____

Paul Hartman

PDI Gage: 297A

Calibration Date: 8/28/2026 6:10:09 AM

Calibration valid 2 years

