




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 356B
PDI Gage Factor: 92.5
Mean Linear Correlation Coefficient: 0.999943

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1953.2	-6.128	647.4	2.053
-1437.0	-4.511	997.4	3.144
-912.1	-2.878	1312.3	4.106
-446.2	-1.409	1627.3	5.051
-164.0	-0.496	2001.3	6.190
229.7	0.737		

Calibration Curve

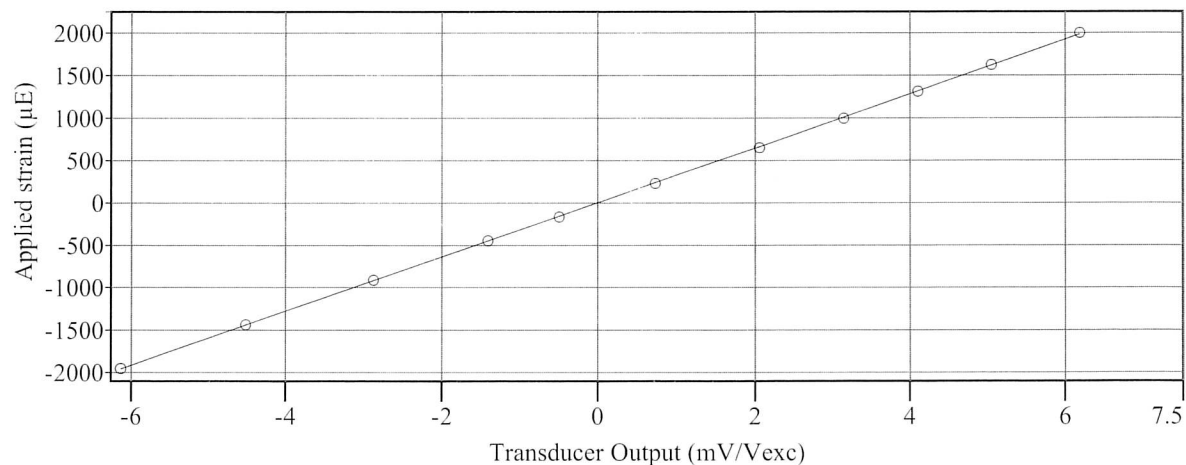

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

PDI Gage: 356B

Calibration Date: _____

Calibration valid 2 years

Signature: _____

Kelly Beal

SEP 15 2026

