




Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 368B
PDI Gage Factor: 93.4
Mean Linear Correlation Coefficient: 0.999916

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1916.0	-5.991	675.9	2.109
-1404.2	-4.389	1036.7	3.209
-879.3	-2.767	1345.1	4.146
-393.7	-1.242	1660.1	5.081
-85.3	-0.270	2001.3	6.080
269.0	0.814		

Calibration Curve

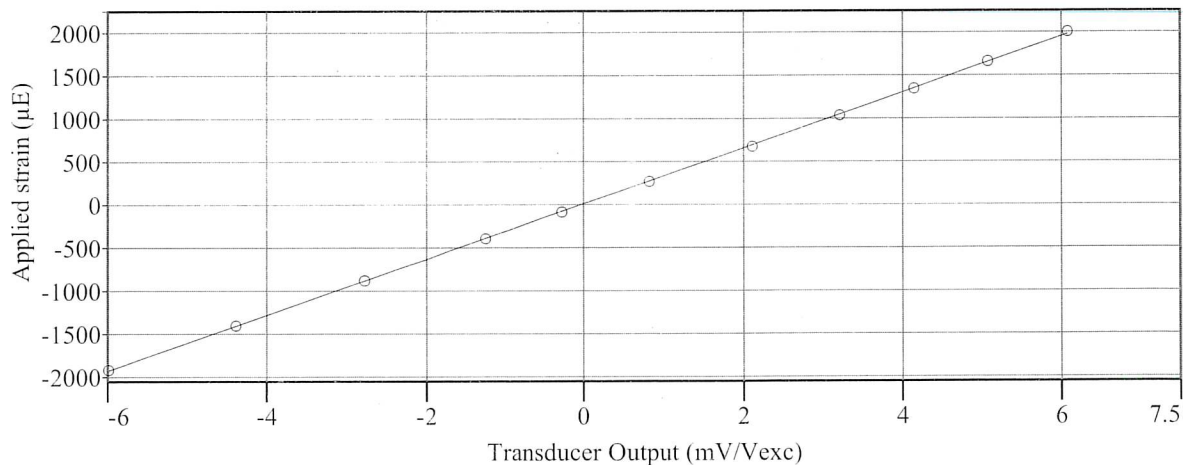

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: 

PDI Gage: 368B

Calibration Date: SEP 15 2026

Calibration valid 2 years

