


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

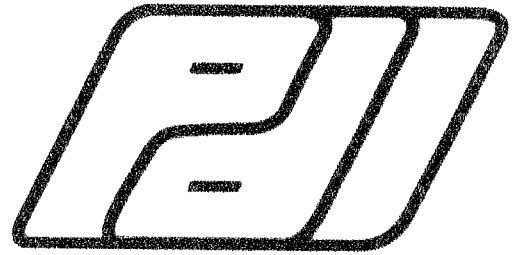

Serial No: 84051 Temperature: 21.4 °C

Model: PIT HAMMER Humidity: 48%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

953.3 g's/volt

R²: 0.999903 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 20Aug2026

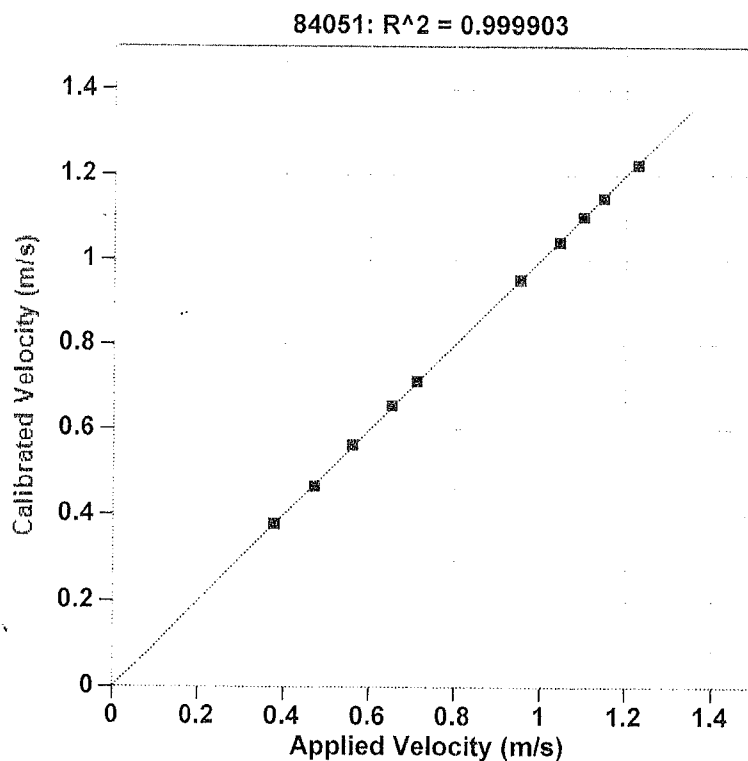

Reference Velocity	S/N 84051 Velocity
m/s	m/s
0.378	0.379
0.470	0.467
0.560	0.564
0.651	0.656
0.711	0.714
0.952	0.953
1.044	1.042
1.100	1.102
1.148	1.145
1.228	1.225
Maximum Acceleration: 231 g's	