


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

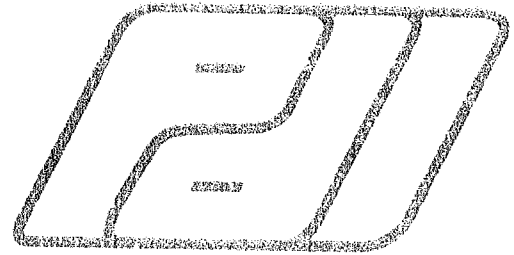

Serial No: K11773 Temperature: 23.8 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

425.2 mv/5000g

(85.0 μ v/g)

R²: 0.999986 [Chip programmed]

Operator: William Johnson

Signed


Calibration valid 2 years

From: 10Aug2026

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

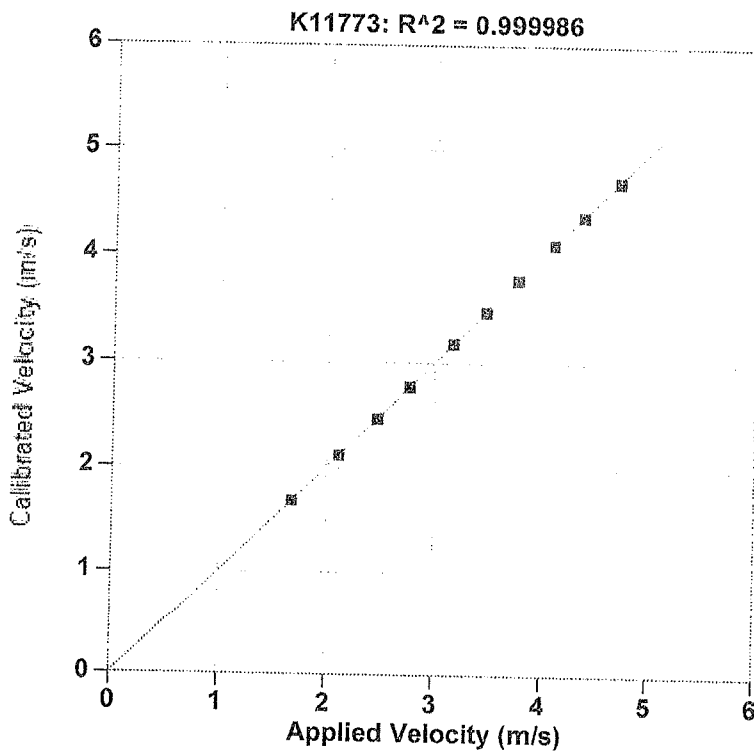

Reference Velocity	S/N K11773 Velocity
m/s	m/s
1.678	1.683
2.114	2.115
2.469	2.464
2.765	2.766
3.173	3.174
3.475	3.472
3.768	3.772
4.103	4.107
4.379	4.374
4.707	4.705

Maximum Acceleration: 1042 g's