


Certificate of Calibration Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

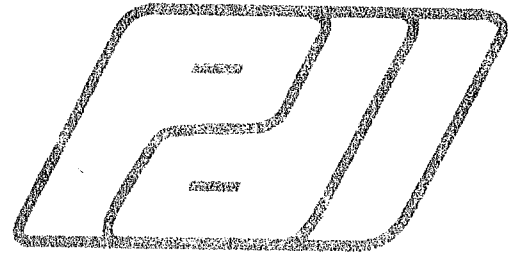

Serial No: K12942 Temperature: 21.8 °C

Model: KICHER PR Humidity: 51%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

345.5 mv/5000g

(69.1 μ v/g)

R²: 0.999948 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson

Signed

Calibration valid 2 years

From: 02Sep2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

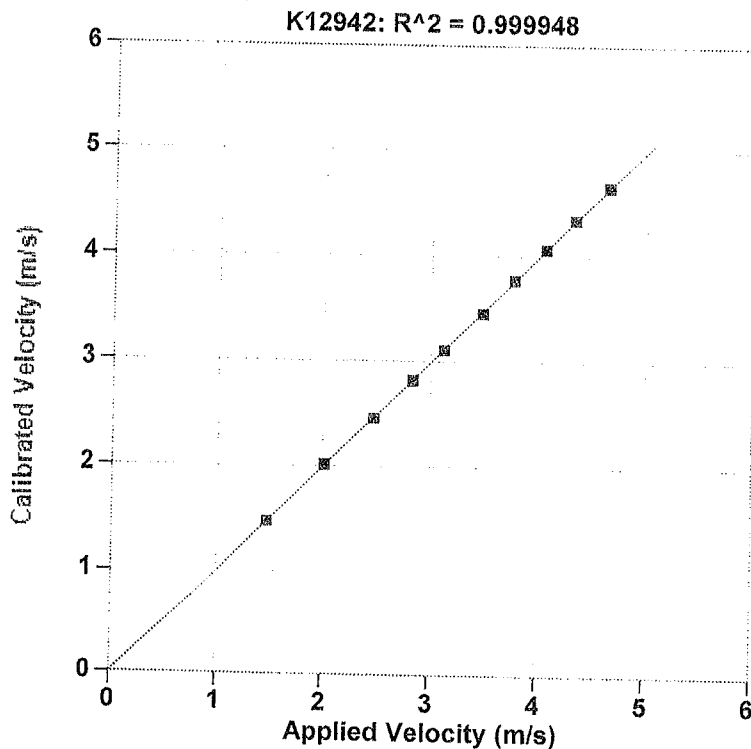

Reference Velocity	S/N K12942 Velocity
m/s	m/s
1.472	1.474
2.014	2.017
2.466	2.458
2.828	2.822
3.118	3.110
3.470	3.458
3.768	3.773
4.062	4.064
4.336	4.344
4.648	4.656

Maximum Acceleration: 1021 g's