

Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15226 Temperature: 22.3 °C
Model: KICHER PR Humidity: 32%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

396.1 mv/5000g
(79.2 μv/g)
R^2: 0.999982 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: **AUG 31 2026**

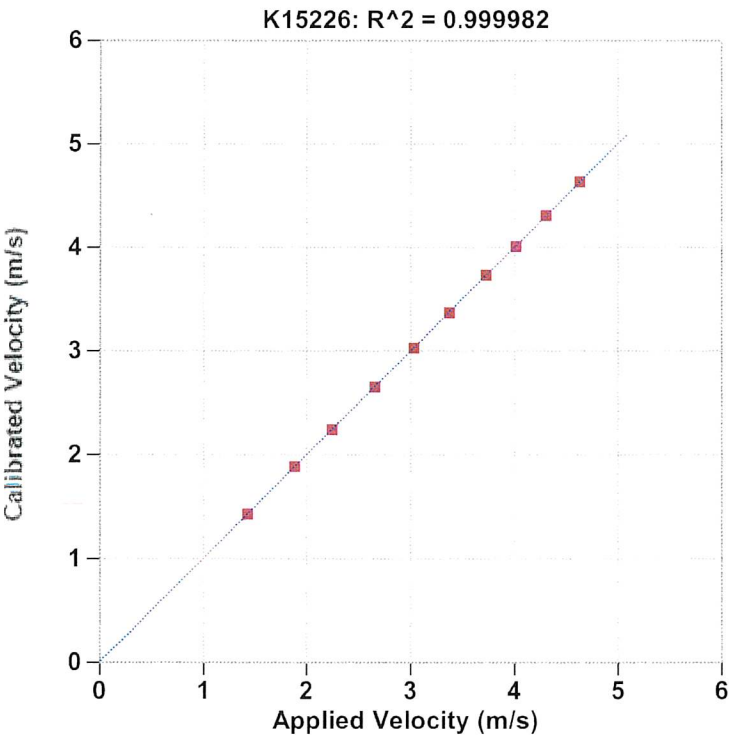

Reference Velocity	S/N K15226 Velocity
m/s	m/s
1.423	1.424
1.880	1.884
2.243	2.237
2.653	2.652
3.027	3.025
3.374	3.368
3.725	3.727
4.010	4.005
4.298	4.302
4.625	4.632

Maximum Acceleration: 1022 g's