

Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.



Serial No: K15525 Temperature: 19.7 °C

Model: KICHER PR Humidity: 49%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

399.4 mv/5000g

(79.9 μ v/g)

R²: 0.999974 [Chip programmed]

Ref Acc 1: 85382! Cal on: 24Nov2025
958 g's/volt

Ref Acc 2: 85363! Cal on: 14Nov2025
1000 g's/volt


Operator: William Johnson


Signed

Reference accelerometer calibrations are traceable to
the United States National Institute of Standards and
Technology (NIST).

Calibration valid 2 years

From: SEP 16 2026

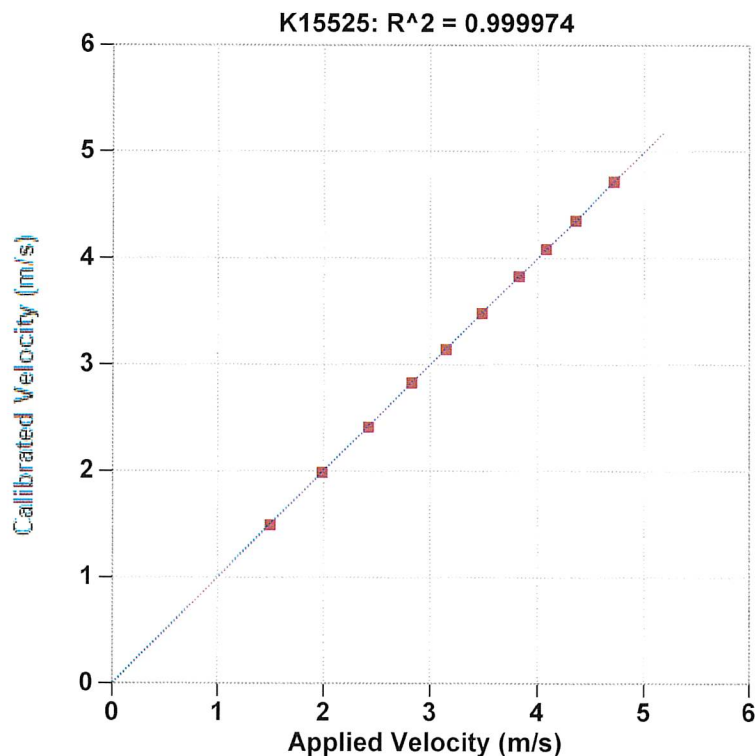

Reference Velocity	S/N K15525 Velocity
m/s	m/s
1.497	1.489
1.984	1.983
2.418	2.409
2.827	2.827
3.147	3.144
3.486	3.482
3.826	3.831
4.079	4.086
4.349	4.354
4.721	4.719

Maximum Acceleration: 1018 g's