


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

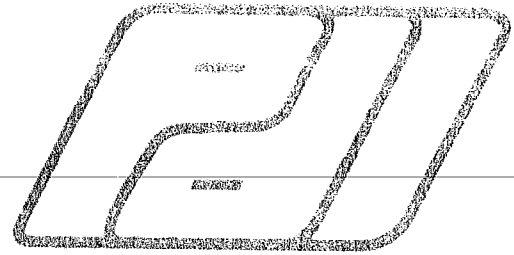

Serial No: K6232 Temperature: 23.8 °C

Model: KICHER PR Humidity: 42%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

363.7 mv/5000g

(72.7 μ v/g)

R²: 0.999986 [Chip programmed]

Operator: William Johnson

Signed


Calibration valid 2 years

From: 10Aug2026

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

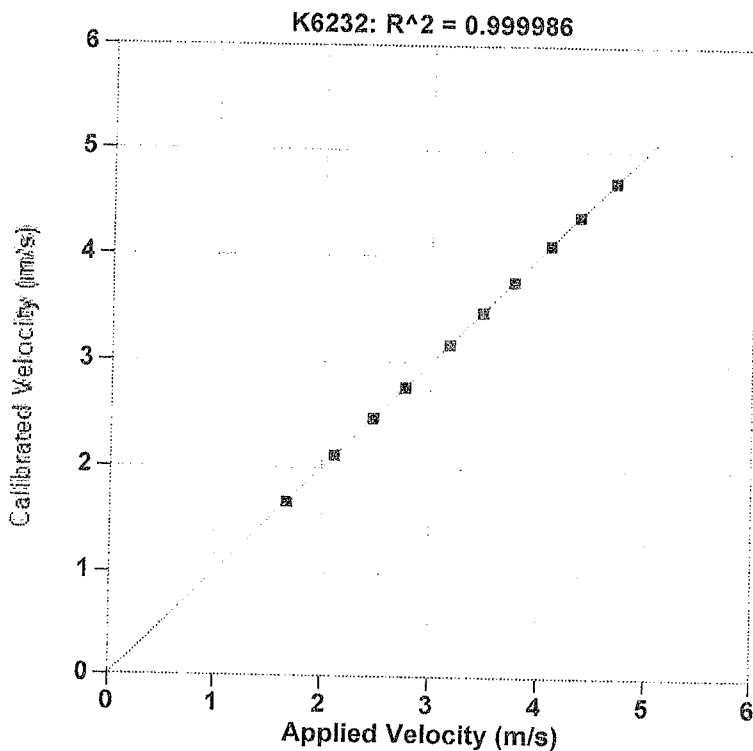

Reference Velocity	S/N K6232 Velocity
m/s	m/s
1.678	1.673
2.114	2.114
2.469	2.471
2.765	2.761
3.173	3.166
3.475	3.475
3.768	3.766
4.103	4.104
4.379	4.381
4.707	4.713
Maximum Acceleration: 1042 g's	