


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

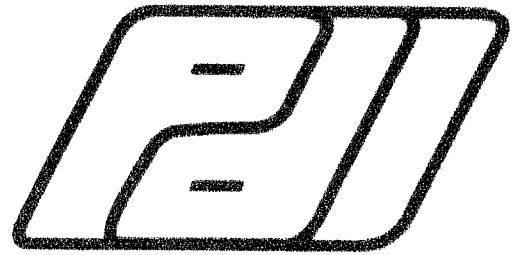

Serial No: LW358418 Temperature: 21.4 °C

Model: PIT ACC Humidity: 48%

Calibrated on: Channel 3 on 8G 5161 LE

PDA CALIBRATION FACTOR

9.8 g's/volt

R²: 0.999925 [No chip]

Ref Acc 1: LW547723! Cal on: 21Oct2025
10 g's/volt

Ref Acc 2: LW547722! Cal on: 21Oct2025
10 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: 20Aug2026

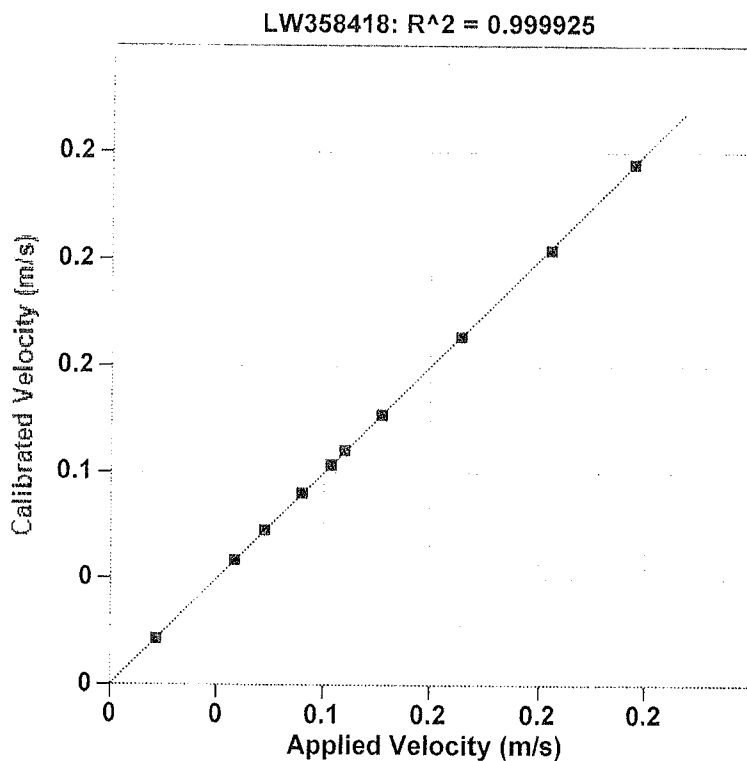

Reference Velocity	S/N LW358418 Velocity
m/s	m/s
0.021	0.021
0.058	0.059
0.072	0.073
0.090	0.091
0.103	0.104
0.110	0.111
0.127	0.127
0.164	0.164
0.206	0.204
0.244	0.245
Maximum Acceleration: 29 g's	