




Certificate of Calibration

Pile Dynamics, Inc.
 Transducer Model: PDI Strain Transducer
 Serial Number: W668
 PDI Gage Factor: 94.1
 Mean Linear Correlation Coefficient: 0.999848

Table 1: Representative Calibration Data

Applied strain (μE)	Gage Output (mV/Vexc)	Applied strain (μE)	Gage Output (mV/Vexc)
-1929.1	-6.042	524.9	1.533
-1450.1	-4.531	885.8	2.640
-958.0	-3.070	1240.2	3.737
-481.2	-1.689	1603.2	4.805
-111.5	-0.500	1975.1	5.886
203.4	0.549		

Calibration Curve

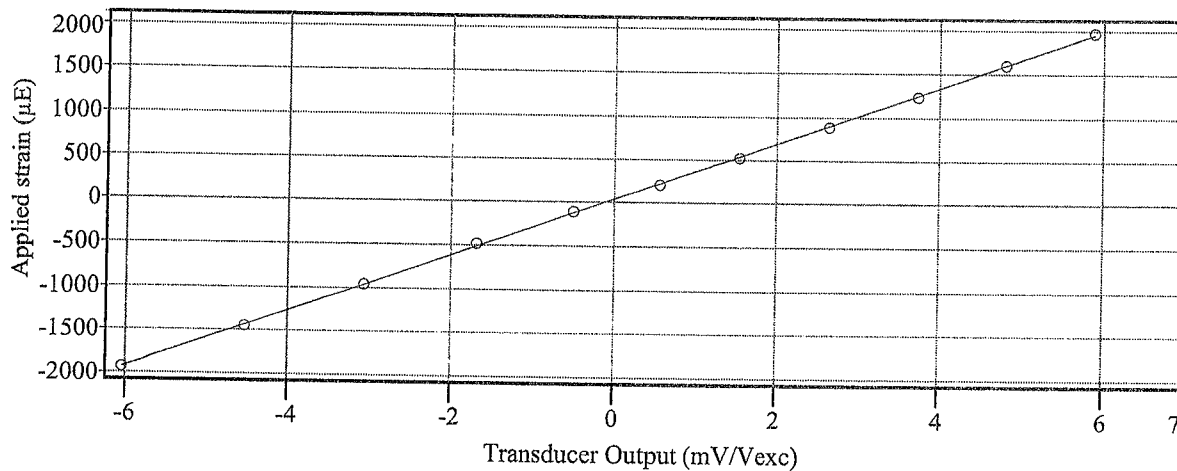

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1006HA
Firmware version number:	0.9.1.1
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Paul Hartman

PDI Gage: W668

Calibration Date: 8/10/2026 7:17:10 AM

Calibration valid 2 years

Signature: _____

Paul Hartman

