


Certificate of Calibration

Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

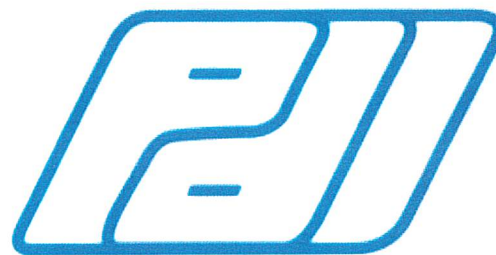

Serial No: 00044 Temperature: 23.5 °C

Model: PR Humidity: 45%

Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1133.7 mv/5000g

(226.7 μ v/g)

R²: 0.999970 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt

Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt

Operator: William Johnson


Signed

Calibration valid 2 years

OCT 01 2026

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

From: _____

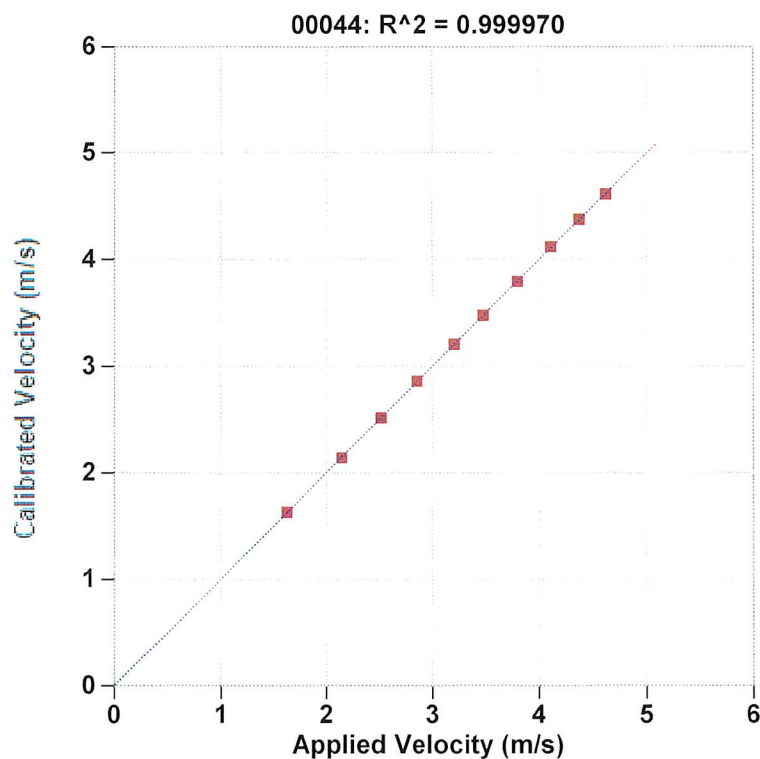

Reference Velocity	S/N 00044 Velocity
m/s	m/s
1.618	1.624
2.143	2.136
2.511	2.511
2.849	2.856
3.203	3.204
3.476	3.477
3.800	3.794
4.111	4.119
4.377	4.377
4.621	4.614

Maximum Acceleration: 990 g's