


Certificate of Calibration
Pile Dynamics, Inc.

Calibrated by Pile Dynamics, Inc.

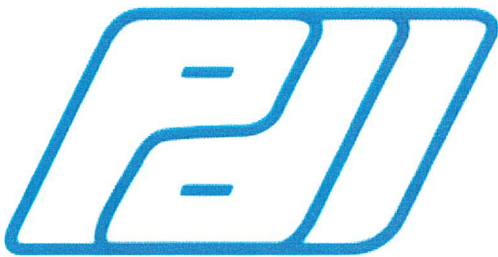

Serial No: 00047 Temperature: 23.5 °C
Model: PR Humidity: 45%
Calibrated on: Channel 4 on 8G 5161 LE

PDA CALIBRATION FACTOR

1154.0 mv/5000g
(230.8 μv/g)
R^2: 0.999951 [Chip programmed]

Ref Acc 1: 85363! Cal on: 14Nov2025
1000 g's/volt
Ref Acc 2: 85382! Cal on: 24Nov2025
958 g's/volt


Operator: William Johnson

William Johnson
Signed

Reference accelerometer calibrations are traceable to the United States National Institute of Standards and Technology (NIST).

Calibration valid 2 years

From: OCT 01 2026

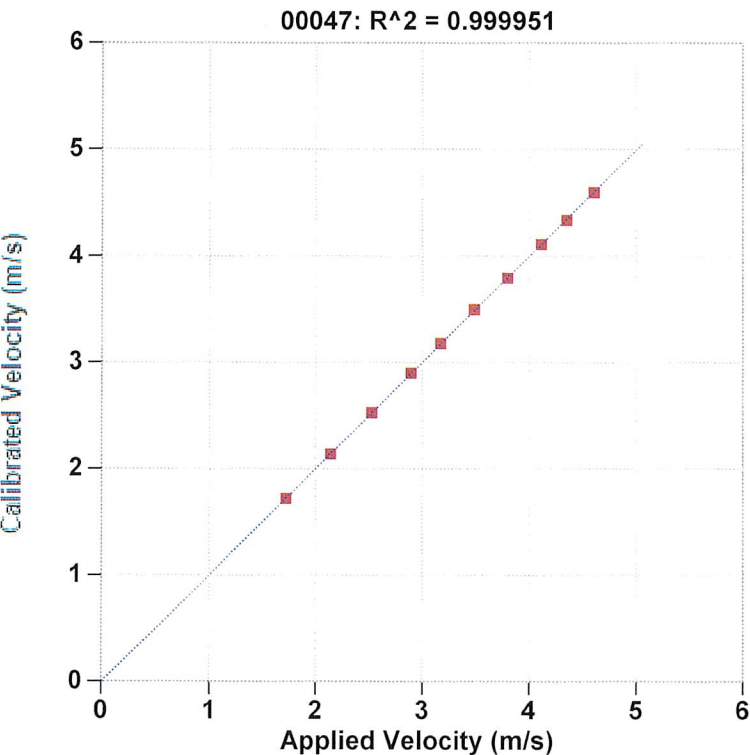

Reference Velocity	S/N 00047 Velocity
m/s	m/s
1.717	1.720
2.139	2.140
2.520	2.526
2.890	2.898
3.171	3.178
3.487	3.495
3.799	3.796
4.110	4.108
4.352	4.340
4.607	4.601

Maximum Acceleration: 979 g's