
# Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 004D
PDI Gage Factor: 90.5
Mean Linear Correlation Coefficient: 0.999956

Table 1: Representative Calibration Data

| Applied strain (μE) | Gage Output (mV/Vexc) | Applied strain (μE) | Gage Output (mV/Vexc) |
|---|---|---|---|
| -1850.4 | -5.851 | 623.4 | 2.047 |
| -1338.6 | -4.228 | 925.2 | 3.026 |
| -839.9 | -2.629 | 1213.9 | 3.968 |
| -433.1 | -1.357 | 1515.7 | 4.924 |
| -142.2 | -0.417 | 1837.3 | 5.900 |
| 255.9 | 0.862 | 2027.6 | 6.467 |

Calibration Curve

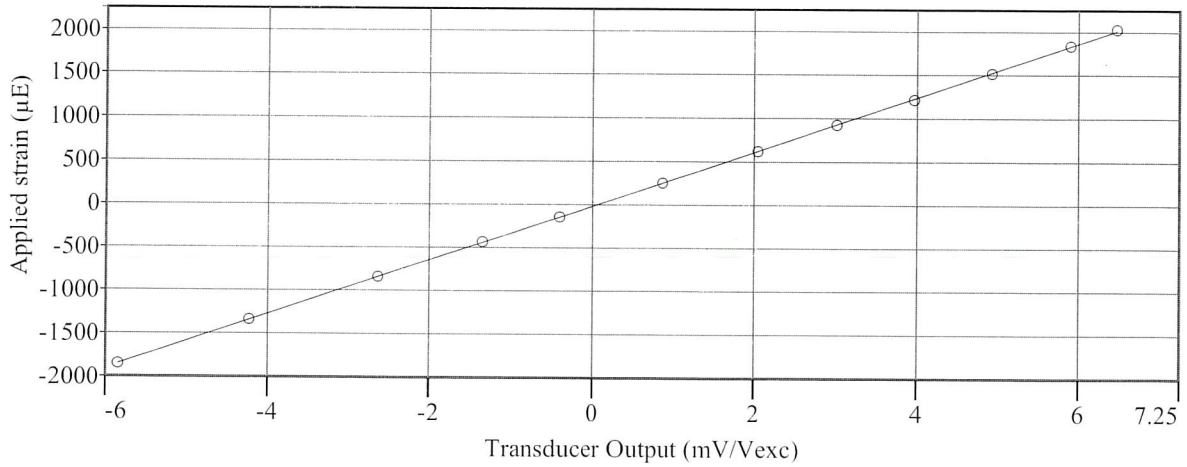


PDI Strain Transducer Calibration System (PDI STCS)

| | |
|---|---|
| PDI STCS Serial Number: | 1000HA |
| Firmware version number: | 0.9.0.0 |
| Transducer Gage Length: | 3 inches (76.2mm) |
| Excitation Voltage for Calibration: | 5.0 VDC |

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal

Signature: Kelly Beal

PDI Gage: 004D

Calibration Date: OCT 2 2 2026

Calibration valid 2 years

Pile Dynamics, Inc.