Certificate of Calibration

Pile Dynamics, Inc.
Transducer Model: PDI Strain Transducer
Serial Number: 013D
PDI Gage Factor: 93.6
Mean Linear Correlation Coefficient: 0.999938

Table 1: Representative Calibration Data

Applied strain (με)	Gage Output (mV/Vexc)	Applied strain (με)	Gage Output (mV/Vexc)
-2040.7	-6.261	621.2	1.960
-1456.7	-4.482	951.4	2.994
-899.0	-2.784	1299.2	4.049
-531.5	-1.643	1640.4	5.100
-78.7	-0.253	2027.6	6.209
301.8	0.937		

Calibration Curve

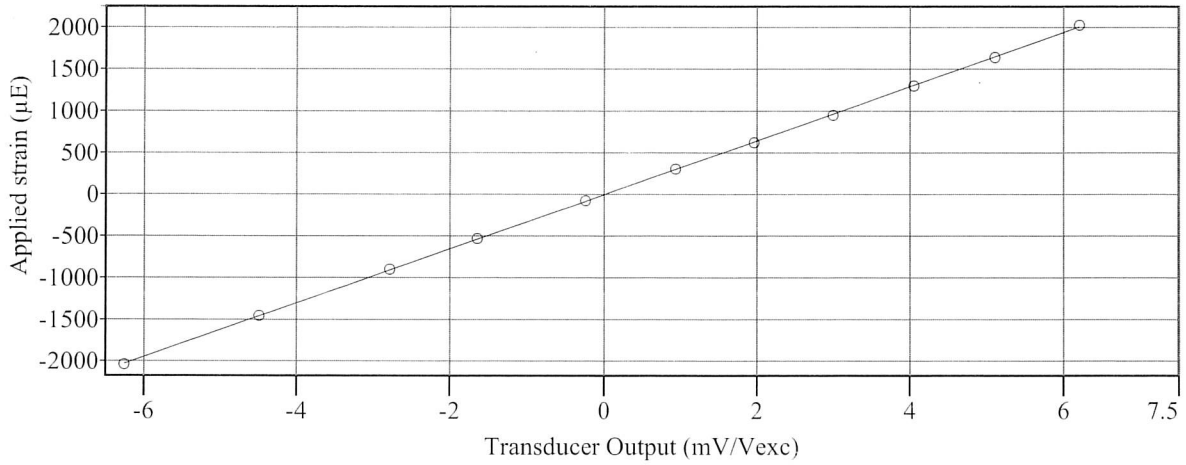

PDI Strain Transducer Calibration System (PDI STCS)

PDI STCS Serial Number:	1000HA
Firmware version number:	0.9.0.0
Transducer Gage Length:	3 inches (76.2mm)
Excitation Voltage for Calibration:	5.0 VDC

PDI certifies the above STCS instrument meets or exceeds published specifications and has been verified using standards and instruments whose accuracies are traceable to the National Institute of Standards and Technology (NIST), an accepted value of a natural physical constant or a ratio calibration technique.

Calibrated By: Kelly Beal Signature: Kelly Beal

PDI Gage: 013D
Calibration Date: OCT 15 2026
Calibration valid 2 years

Pile Dynamics, Inc.